


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA_G\Data\BG011518\
Data File : BG032049.D
Acq On : 16 Jan 2018 2:21
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG011218.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Jan 15 10:05:15 2018

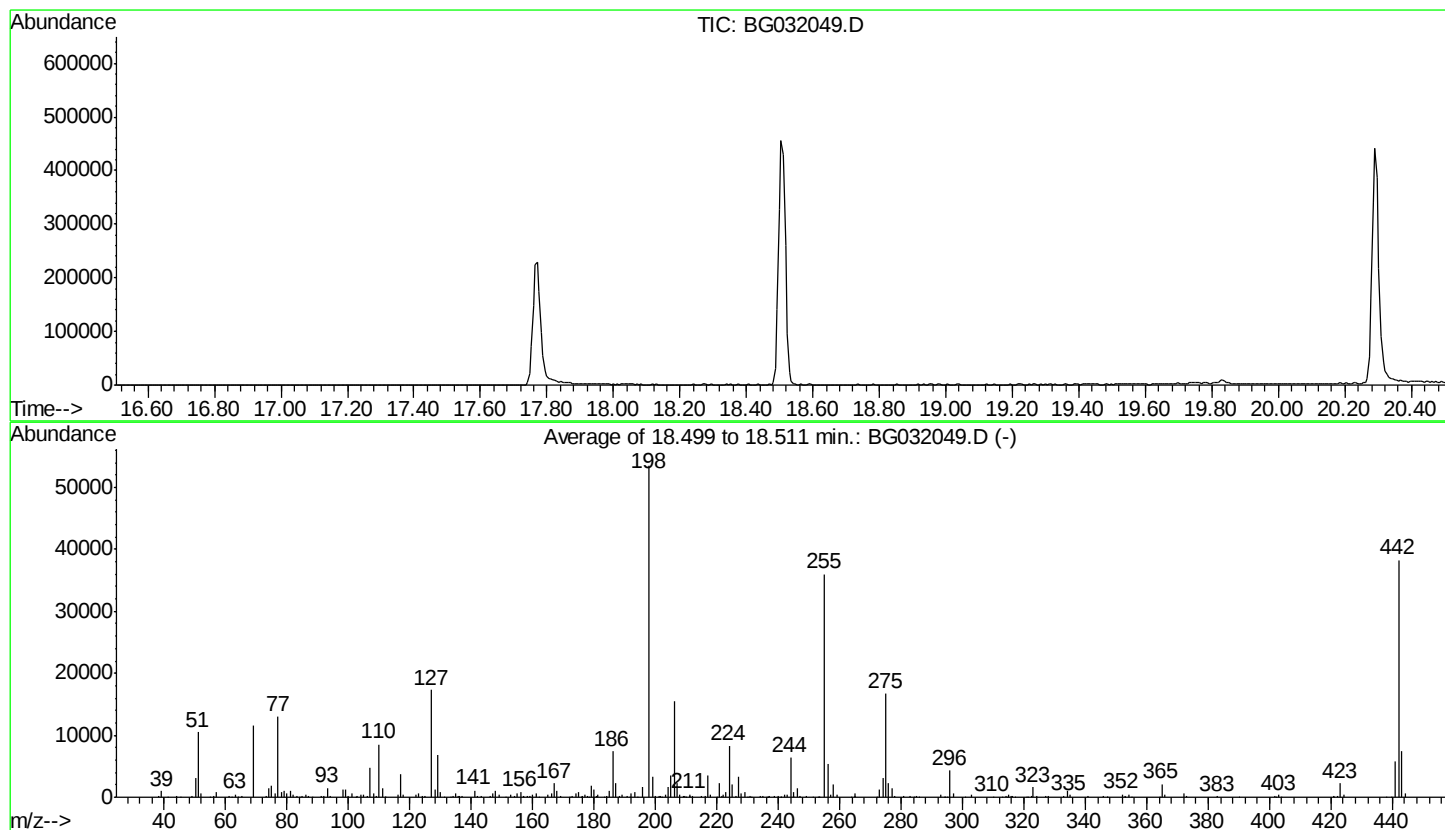

AutoFind: Scans 2589, 2590, 2591; Background Corrected with Scan 2583

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	19.7	10534	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	21.5	11509	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	32.3	17302	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	53509	PASS
199	198	5	9	6.4	3408	PASS
275	198	10	60	31.3	16728	PASS
365	198	1	100	3.9	2079	PASS
441	442	0.01	24	15.0	5732	PASS
442	198	50	100	71.5	38266	PASS
443	442	15	24	19.6	7503	PASS