


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG011520\
 Data File : BG044050.D
 Acq On : 15 Jan 2020 14:58
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG123019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 31 13:32:23 2019

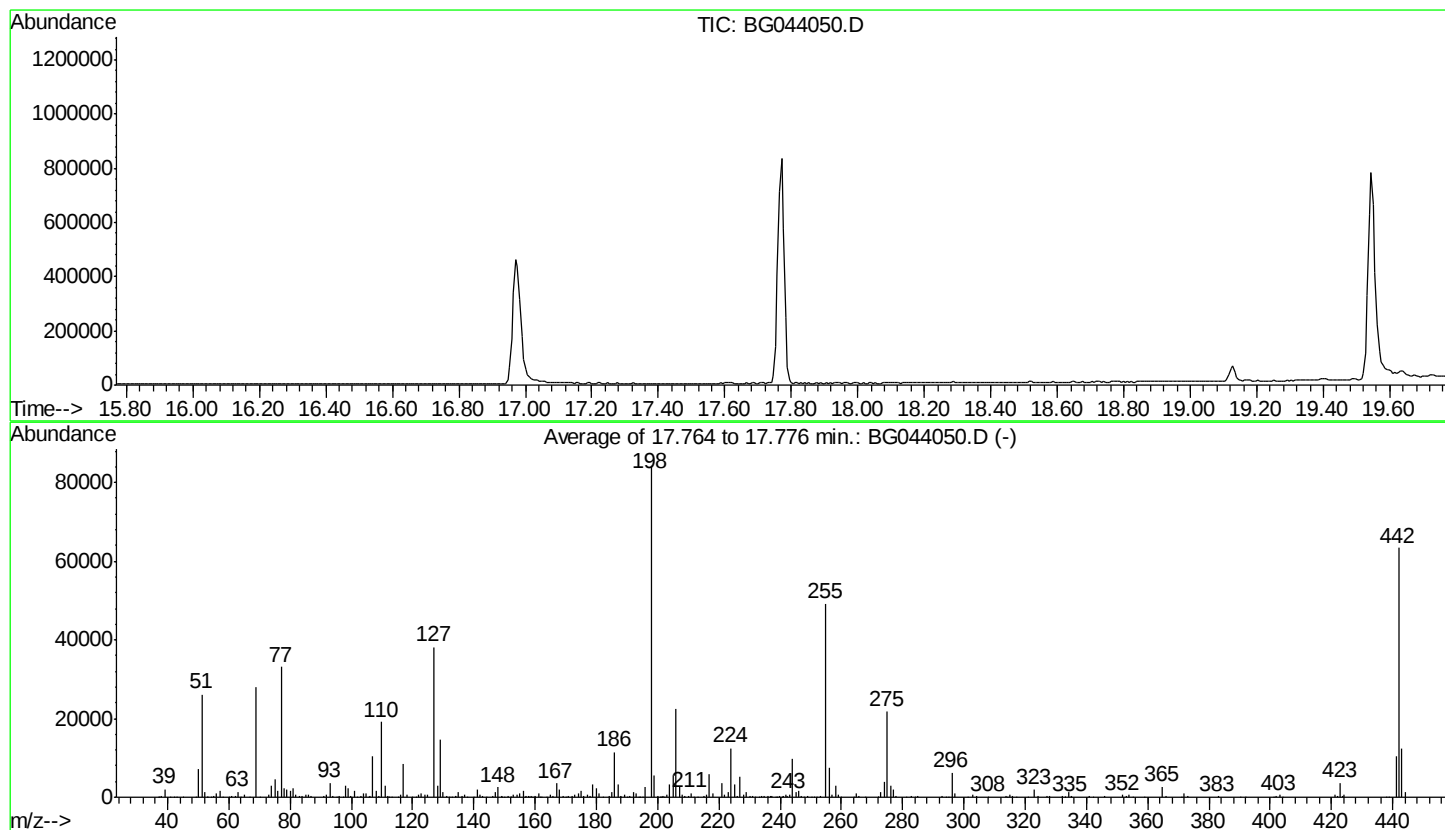

AutoFind: Scans 2498, 2499, 2500; Background Corrected with Scan 2491

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.0	26144	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	33.3	28103	PASS
70	69	0.00	2	0.4	104	PASS
127	198	10	80	45.2	38122	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	84290	PASS
199	198	5	9	6.7	5629	PASS
275	198	10	60	25.8	21741	PASS
365	198	1	100	3.1	2654	PASS
441	198	0.01	100	12.3	10334	PASS
442	198	50	100	75.1	63306	PASS
443	442	15	24	19.7	12495	PASS