




Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG011521\
Data File : BG047923.D
Acq On : 15 Jan 2021 13:38
Operator : CG/JU
Sample : SST00505
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SST005005

Manual Integrations
APPROVED

mohammad
1/18/2021 3:35:52 PM

Quant Time: Jan 15 15:43:31 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG011521.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 15 15:35:35 2021
Response via : Initial Calibration

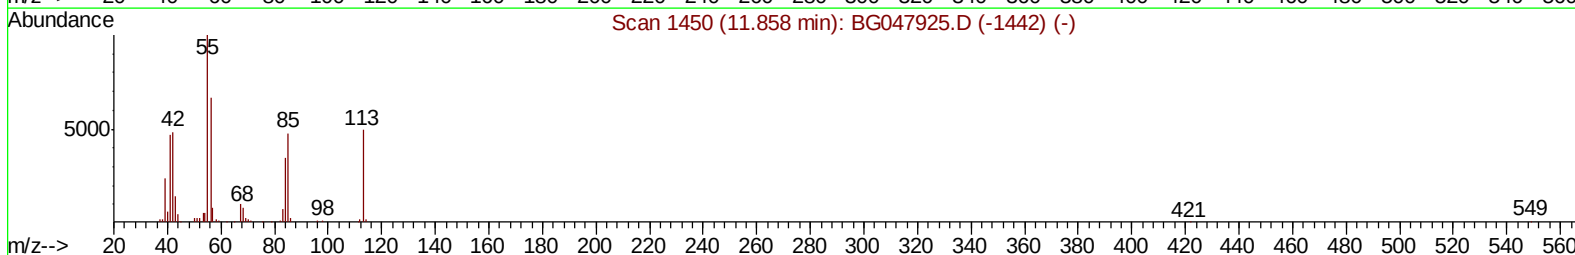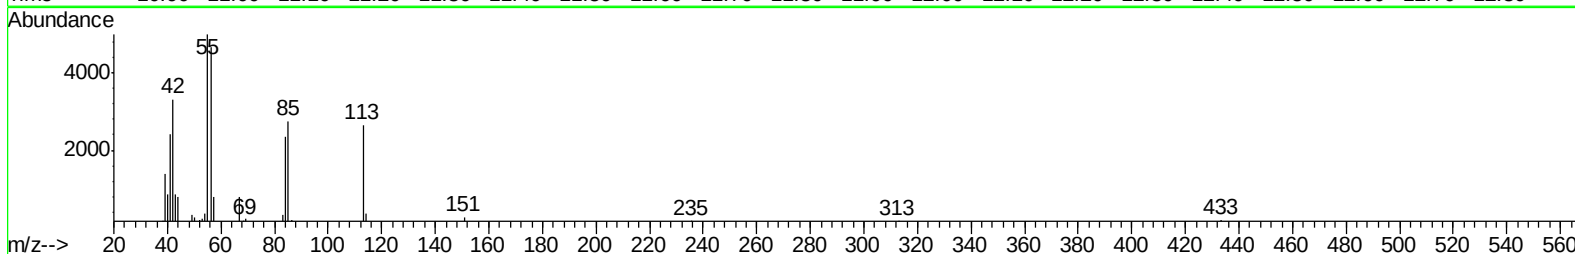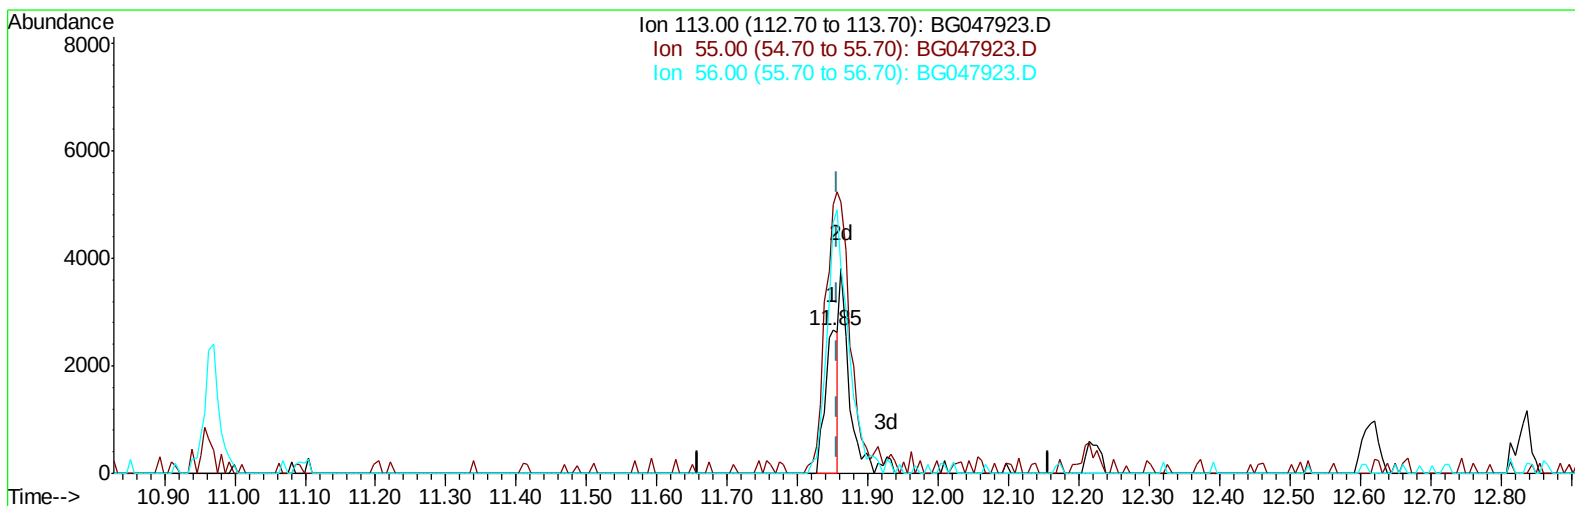

TIC: BG047923.D

(34) Caprolactam

11.850min (-0.008) 2.17ng/ul

response 3434

Ion	Exp%	Act%
113.00	100	100
55.00	202.00	187.90
56.00	135.40	175.21#
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG011521\
Data File : BG047923.D
Acq On : 15 Jan 2021 13:38
Operator : CG/JU
Sample : SST000505
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SSTD005005

Manual Integrations
APPROVED

mohammad
1/18/2021 3:35:52 PM

Quant Time: Jan 15 16:09:33 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SFAM-EPA-BG011521.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 15 15:35:35 2021
Response via : Initial Calibration

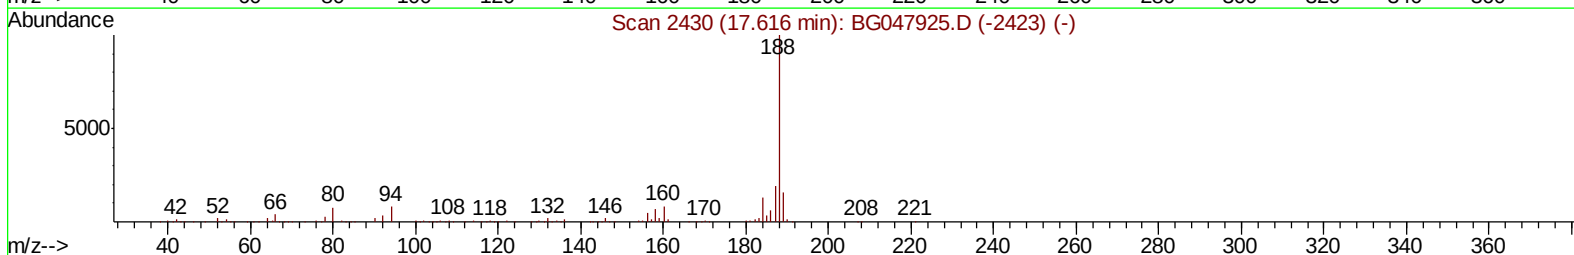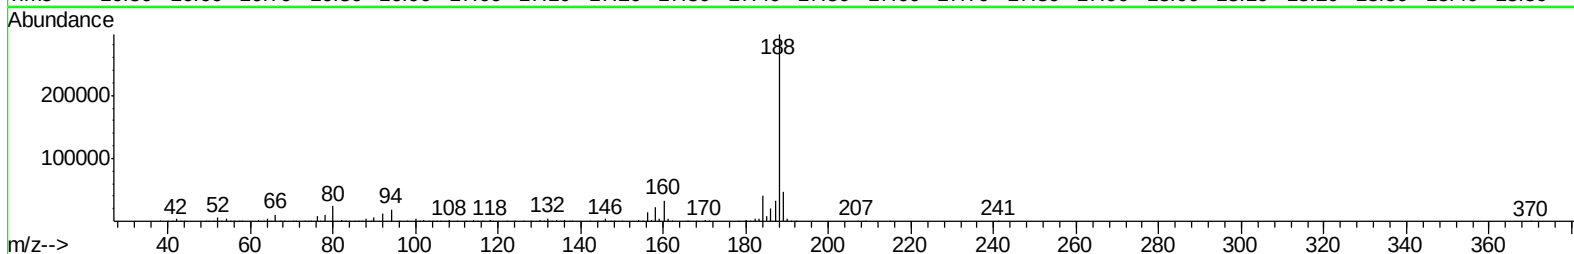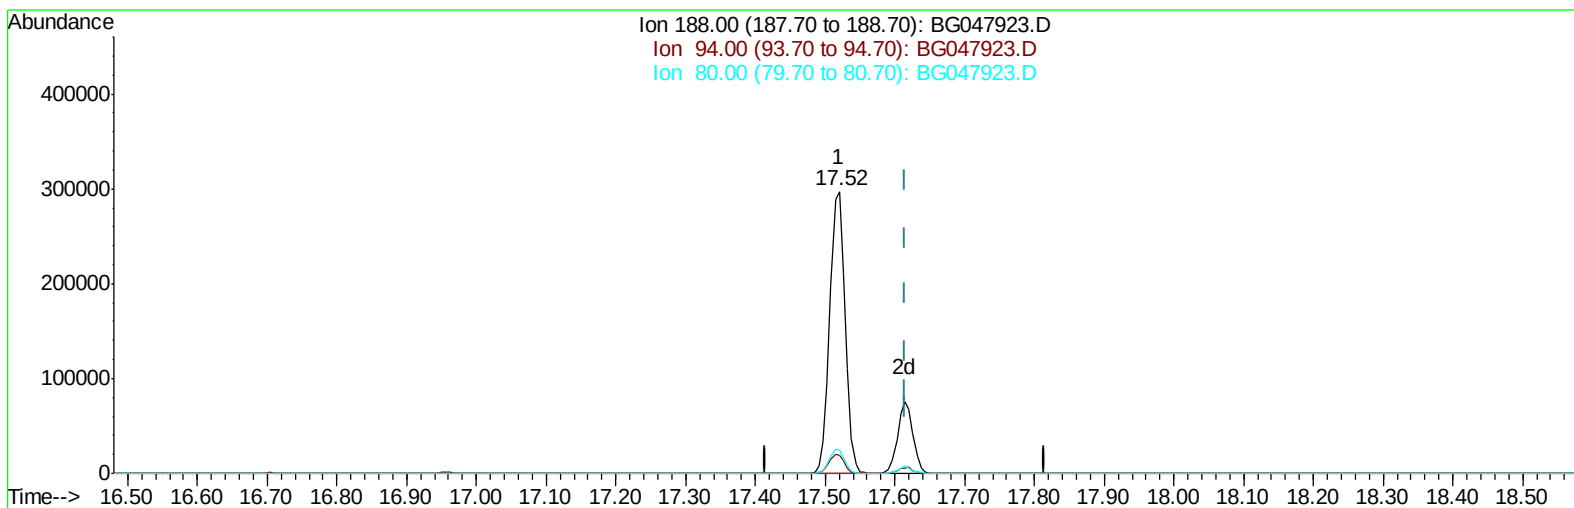

TIC: BG047923.D

(73) Anthracene-d10 (S)

17.520min (-0.096) 20.87ng/ul

response 455967

Ion	Exp%	Act%
188.00	100	100
94.00	8.00	6.41
80.00	7.60	7.98
0.00	0.00	0.00