
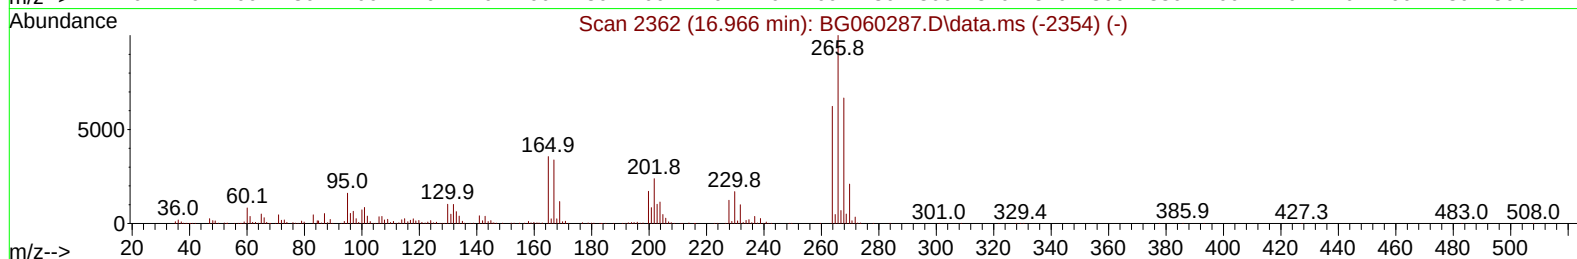
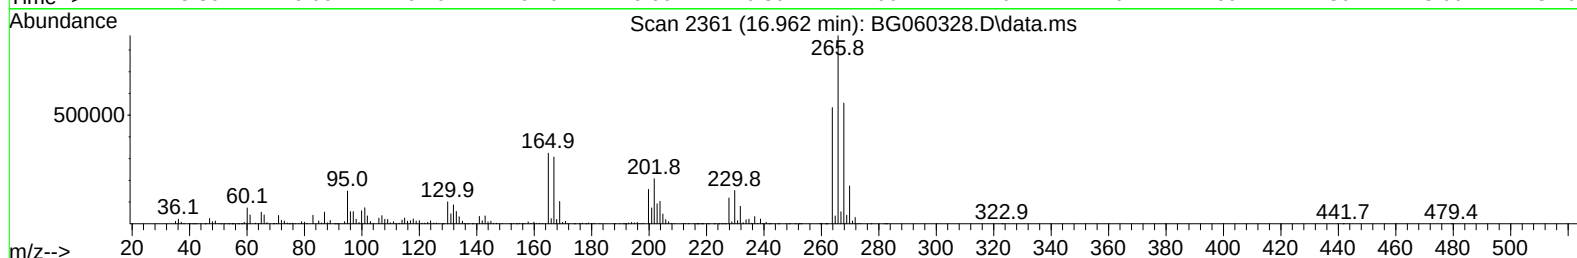


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011524\
Data File : BG060328.D
Acq On : 15 Jan 2024 10:44
Operator : MA/JU
Sample : DFTPP
Misc : 8270 SURROGATES
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 15 19:10:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration

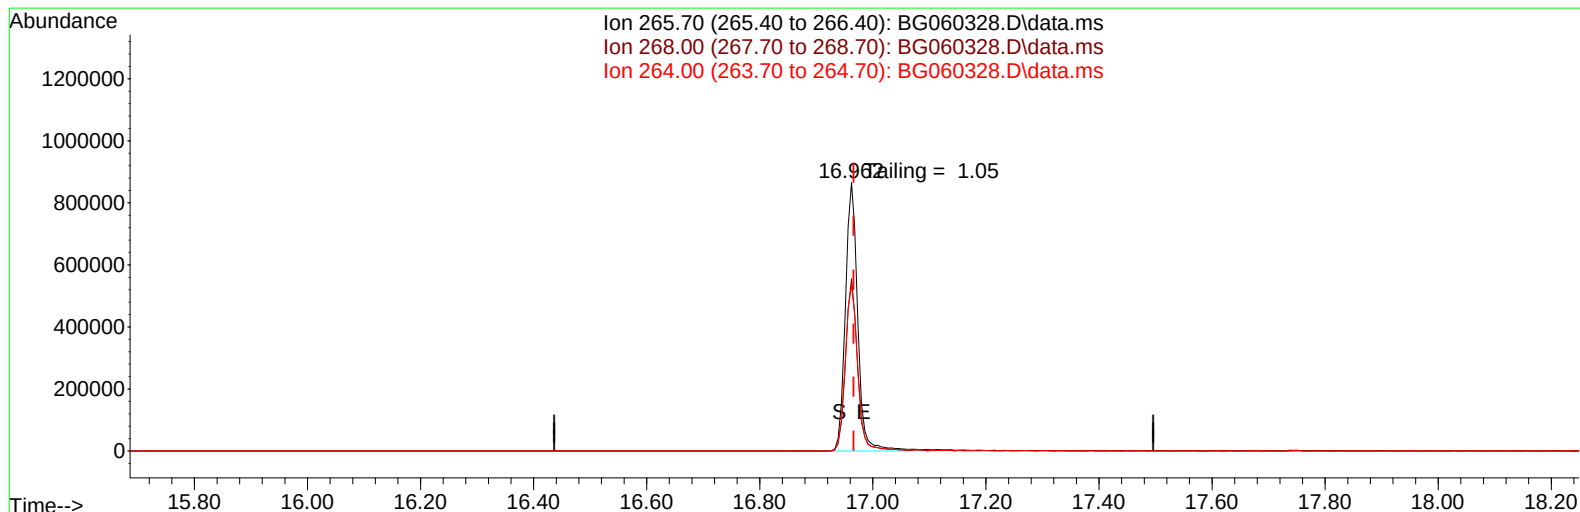




TIC: BG060328.D\data.ms

(70) Pentachlorophenol (C)**16.962min (-0.004) 1608251.98 ng****response 1319197**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	71.80	64.14
264.00	62.30	61.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011524\
Data File : BG060328.D
Acq On : 15 Jan 2024 10:44
Operator : MA/JU
Sample : DFTPP
Misc : 8270 SURROGATES
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 15 19:10:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration

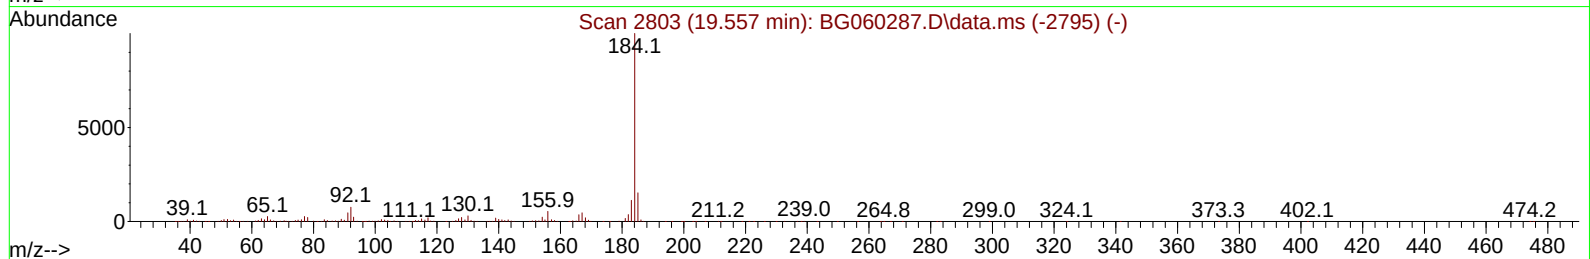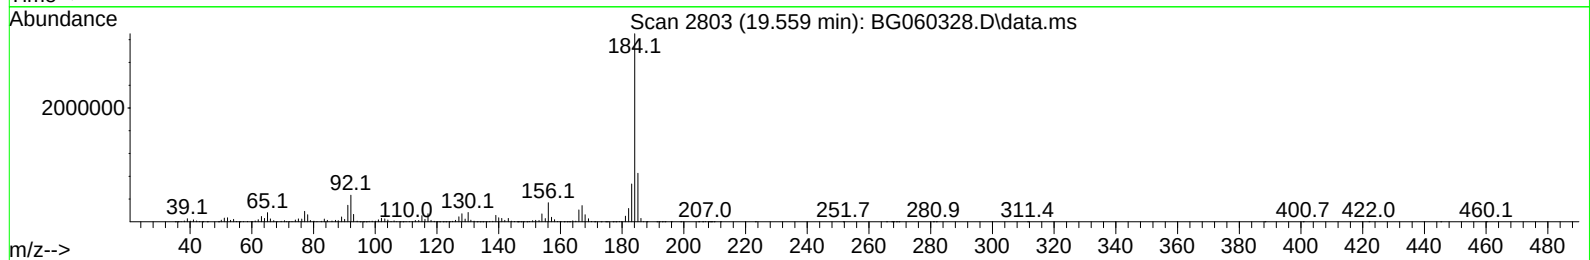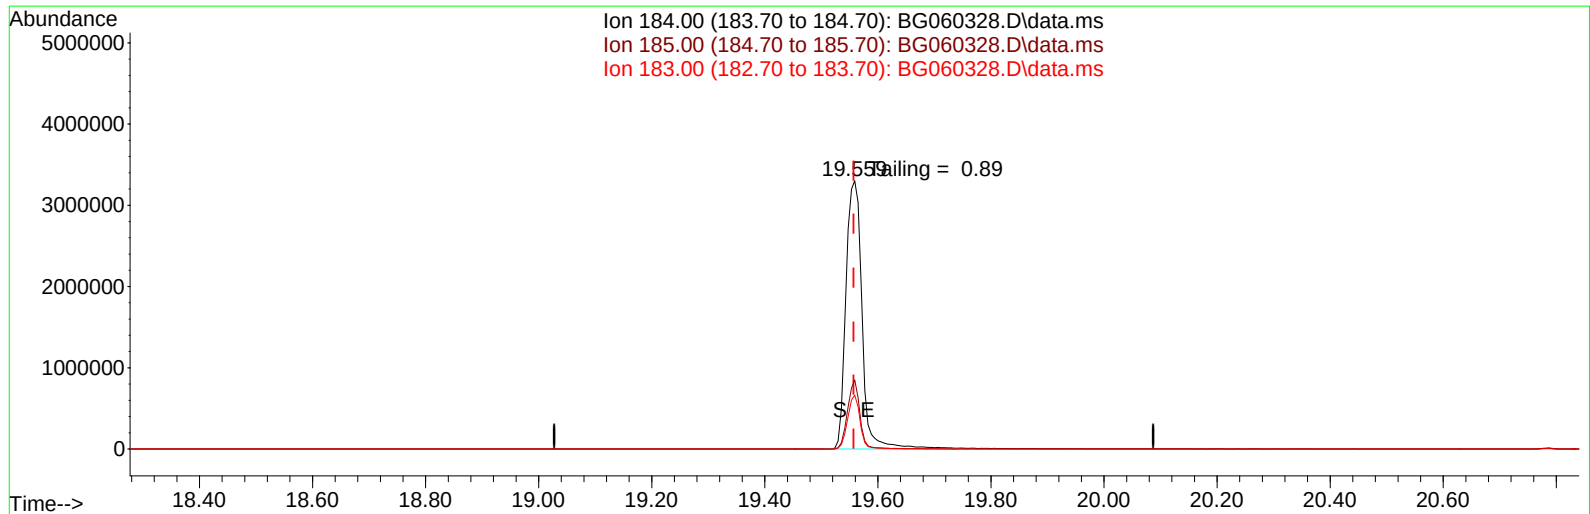

TIC: BG060328.D\data.ms

(77) Benzidine

19.559min (+ 0.002) 0.00 ng

response 6548461

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	25.75#
183.00	11.20	20.11#
0.00	0.00	0.00