
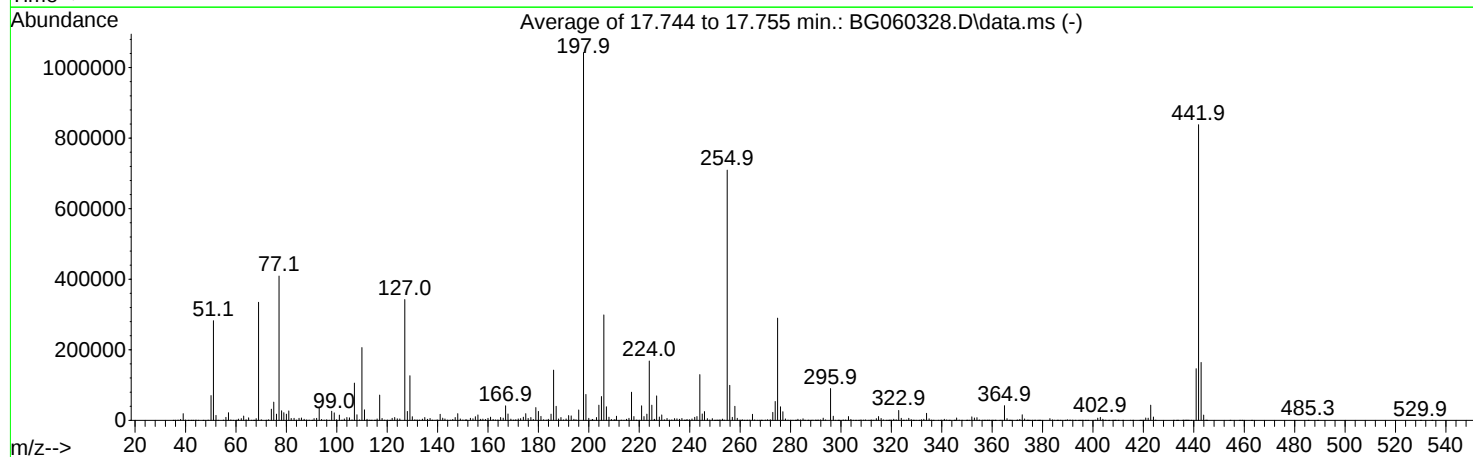


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011524\
Data File : BG060328.D
Acq On : 15 Jan 2024 10:44
Operator : MA/JU
Sample : DFTPP
Misc : 8270 SURROGATES
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jan 09 04:07:12 2024

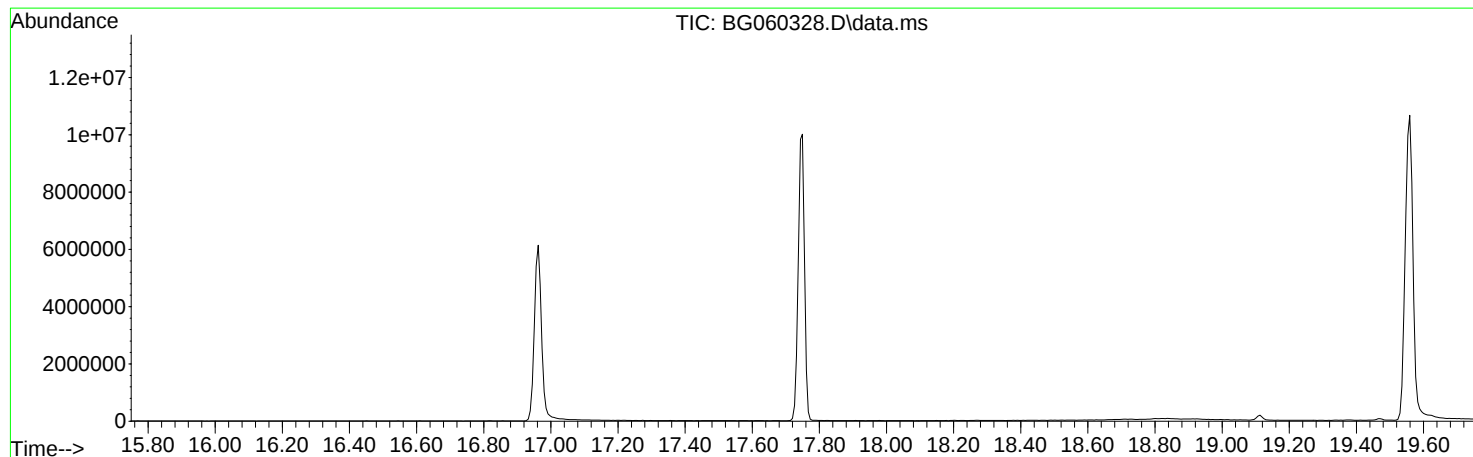




AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2486

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.1	282368	PASS
68	69	0.00	2	1.5	4993	PASS
69	198	0.00	100	32.1	334854	PASS
70	69	0.00	2	0.5	1726	PASS
127	198	10	80	32.8	342379	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	1042816	PASS
199	198	5	9	7.1	73705	PASS
275	198	10	60	27.8	289984	PASS
365	198	1	100	4.0	41853	PASS
441	198	0.01	100	14.0	146395	PASS
442	442	50	100	100.0	838229	PASS
443	442	15	24	19.6	164096	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011524\
Data File : BG060328.D
Acq On : 15 Jan 2024 10:44
Operator : MA/JU
Sample : DFTPP
Misc : 8270 SURROGATES
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 15 19:10:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration

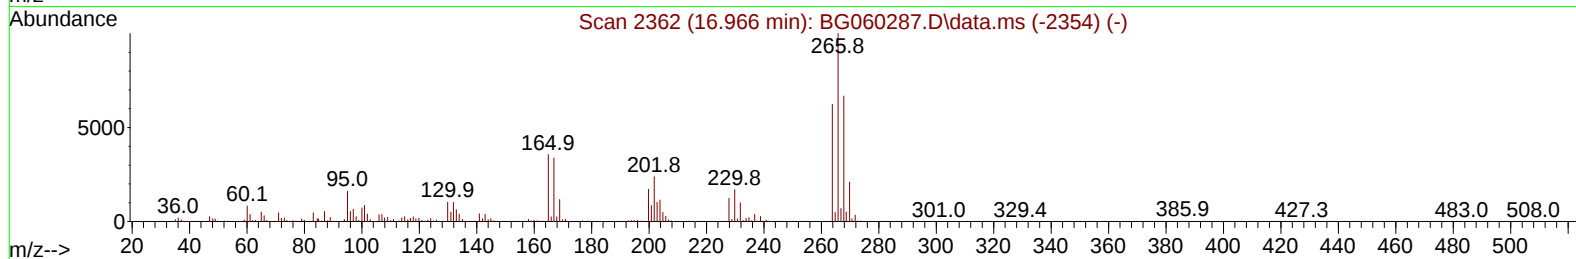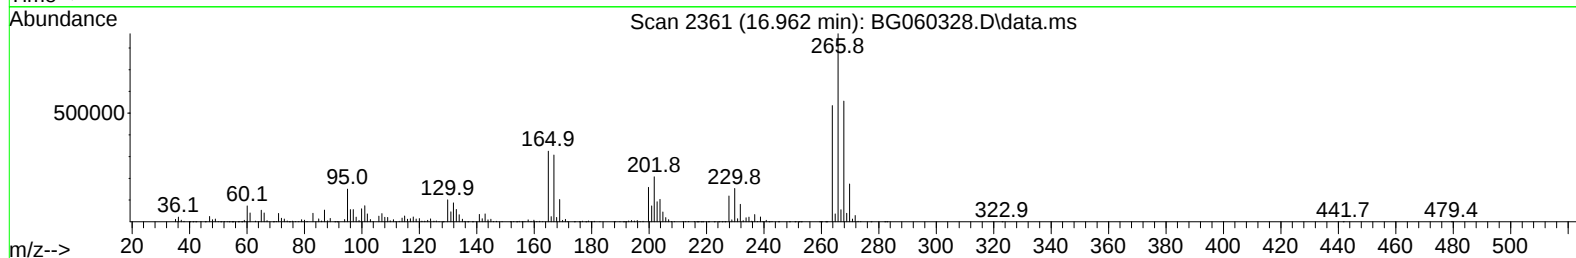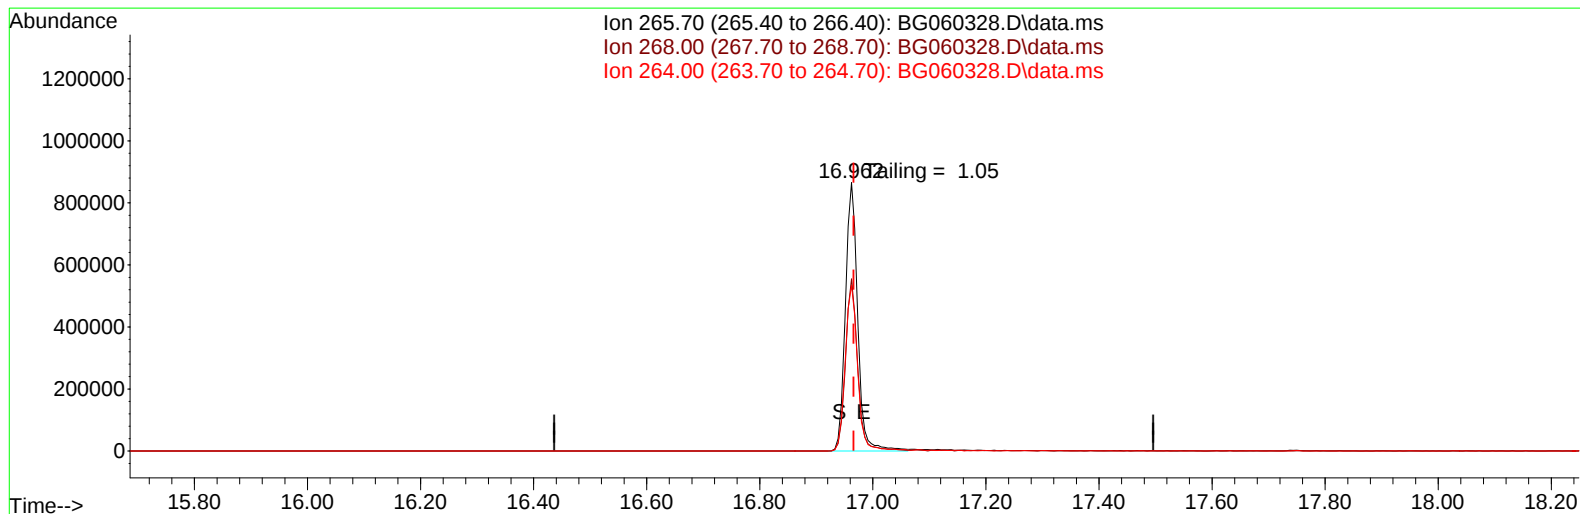

TIC: BG060328.D\data.ms

(70) Pentachlorophenol (C)

16.962min (-0.004) 1608251.98 ng




response 1319197

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	71.80	64.14
264.00	62.30	61.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011524\
Data File : BG060328.D
Acq On : 15 Jan 2024 10:44
Operator : MA/JU
Sample : DFTPP
Misc : 8270 SURROGATES
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 15 19:10:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration

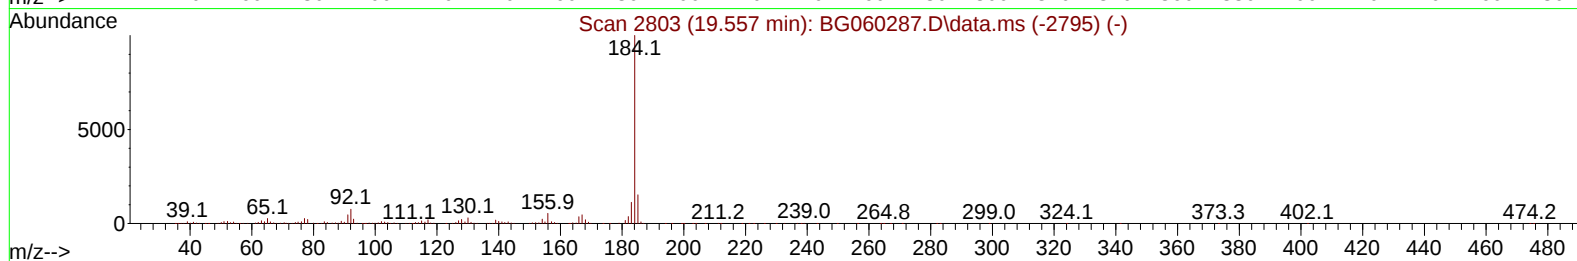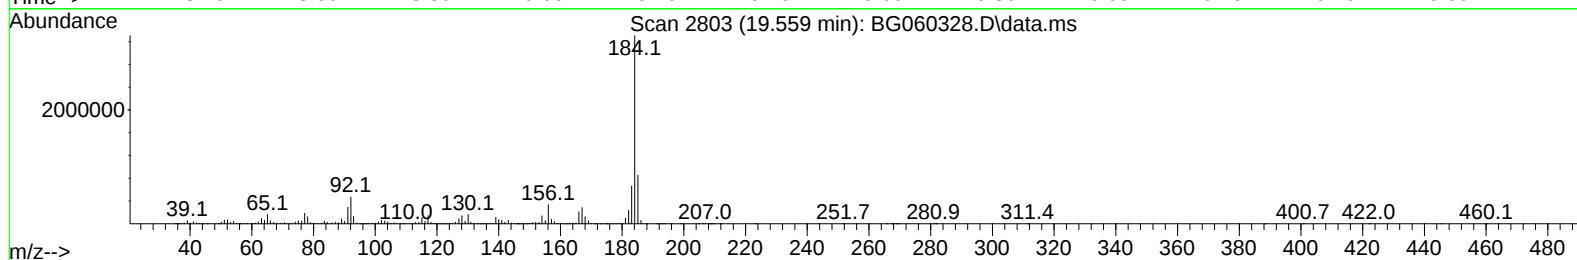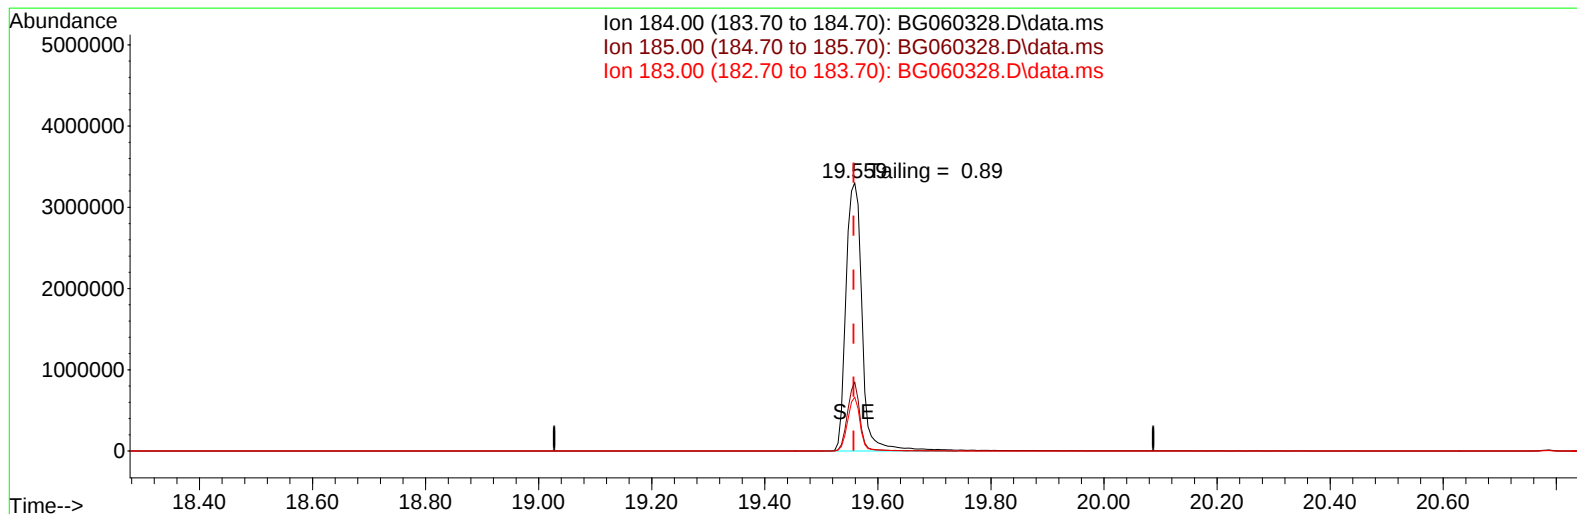

TIC: BG060328.D\data.ms

(77) Benzidine

19.559min (+ 0.002) 0.00 ng

response 6548461

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	25.75#
183.00	11.20	20.11#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/15/2024	BNA_G	<u>BG060328.D</u>
Compound Name	Response	Retention Time
DDT	3570264	20.787
DDD	64731	20.393
DDE	695	19.835
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
65426	3635690	1.80

Instrument :
BNA_G
ClientSampleId :
DFTPP