

Data Path : U:\HPCHEM1\BNA G\DATA\BG011618\  
 Data File : BG032093.D  
 Acq On : 17 Jan 2018 6:05  
 Operator : SJ/JU  
 Sample : J1131-01  
 Misc :  
 ALS Vial : 23 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :

Quant Time: Jan 17 08:07:02 2018  
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\BFDDTBREAKDOWN.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Sep 01 16:14:27 2010  
 Response via : Initial Calibration

| Internal Standards        | R.T.  | QIon | Response | Conc  | Units | Dev(Min) |
|---------------------------|-------|------|----------|-------|-------|----------|
| 1) 1,4-Dichlorobenzene-d4 | 0.00  | 152  | 0        | 0.00  | ng    | -10.26   |
| 2) Naphthalene-d8         | 11.65 | 136  | 190683   | 40.00 | ng    | -0.07    |
| 3) Acenaphthene-d10       | 14.82 | 164  | 2297     | 40.00 | ng    | -0.09    |
| 4) Phenanthrene-d10       | 15.44 | 188  | 65       | 40.00 | ng    | 0.35     |
| 8) Chrysene-d12           | 31.20 | 240  | 54       | 40.00 | ng    | 0.27     |
| 9) Perylene-d12           | 0.00  | 264  | 0        | 0.00  | ng    | -34.56   |


| Target Compounds | R.T. | QIon | Response | Conc | Units | Ovalue |
|------------------|------|------|----------|------|-------|--------|
| 5) DDE           | 0.00 | 246  | 0        | N.D. |       |        |
| 6) DDD           | 0.00 | 235  | 0        | N.D. |       |        |
| 7) DDT           | 0.00 | 235  | 0        | N.D. |       |        |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : U:\HPCHEM1\BNA G\DATA\BG011618\  
Data File : BG032093.D  
Acq On : 17 Jan 2018 6:05  
Operator : SJ/JU  
Sample : J1131-01  
Misc :  
ALS Vial : 23 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :

Quant Time: Jan 17 08:07:02 2018  
Quant Method : Z:\HPCHEM1\BNA F\METHODS\BFDDTBREAKDOWN.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Sep 01 16:14:27 2010  
Response via : Initial Calibration


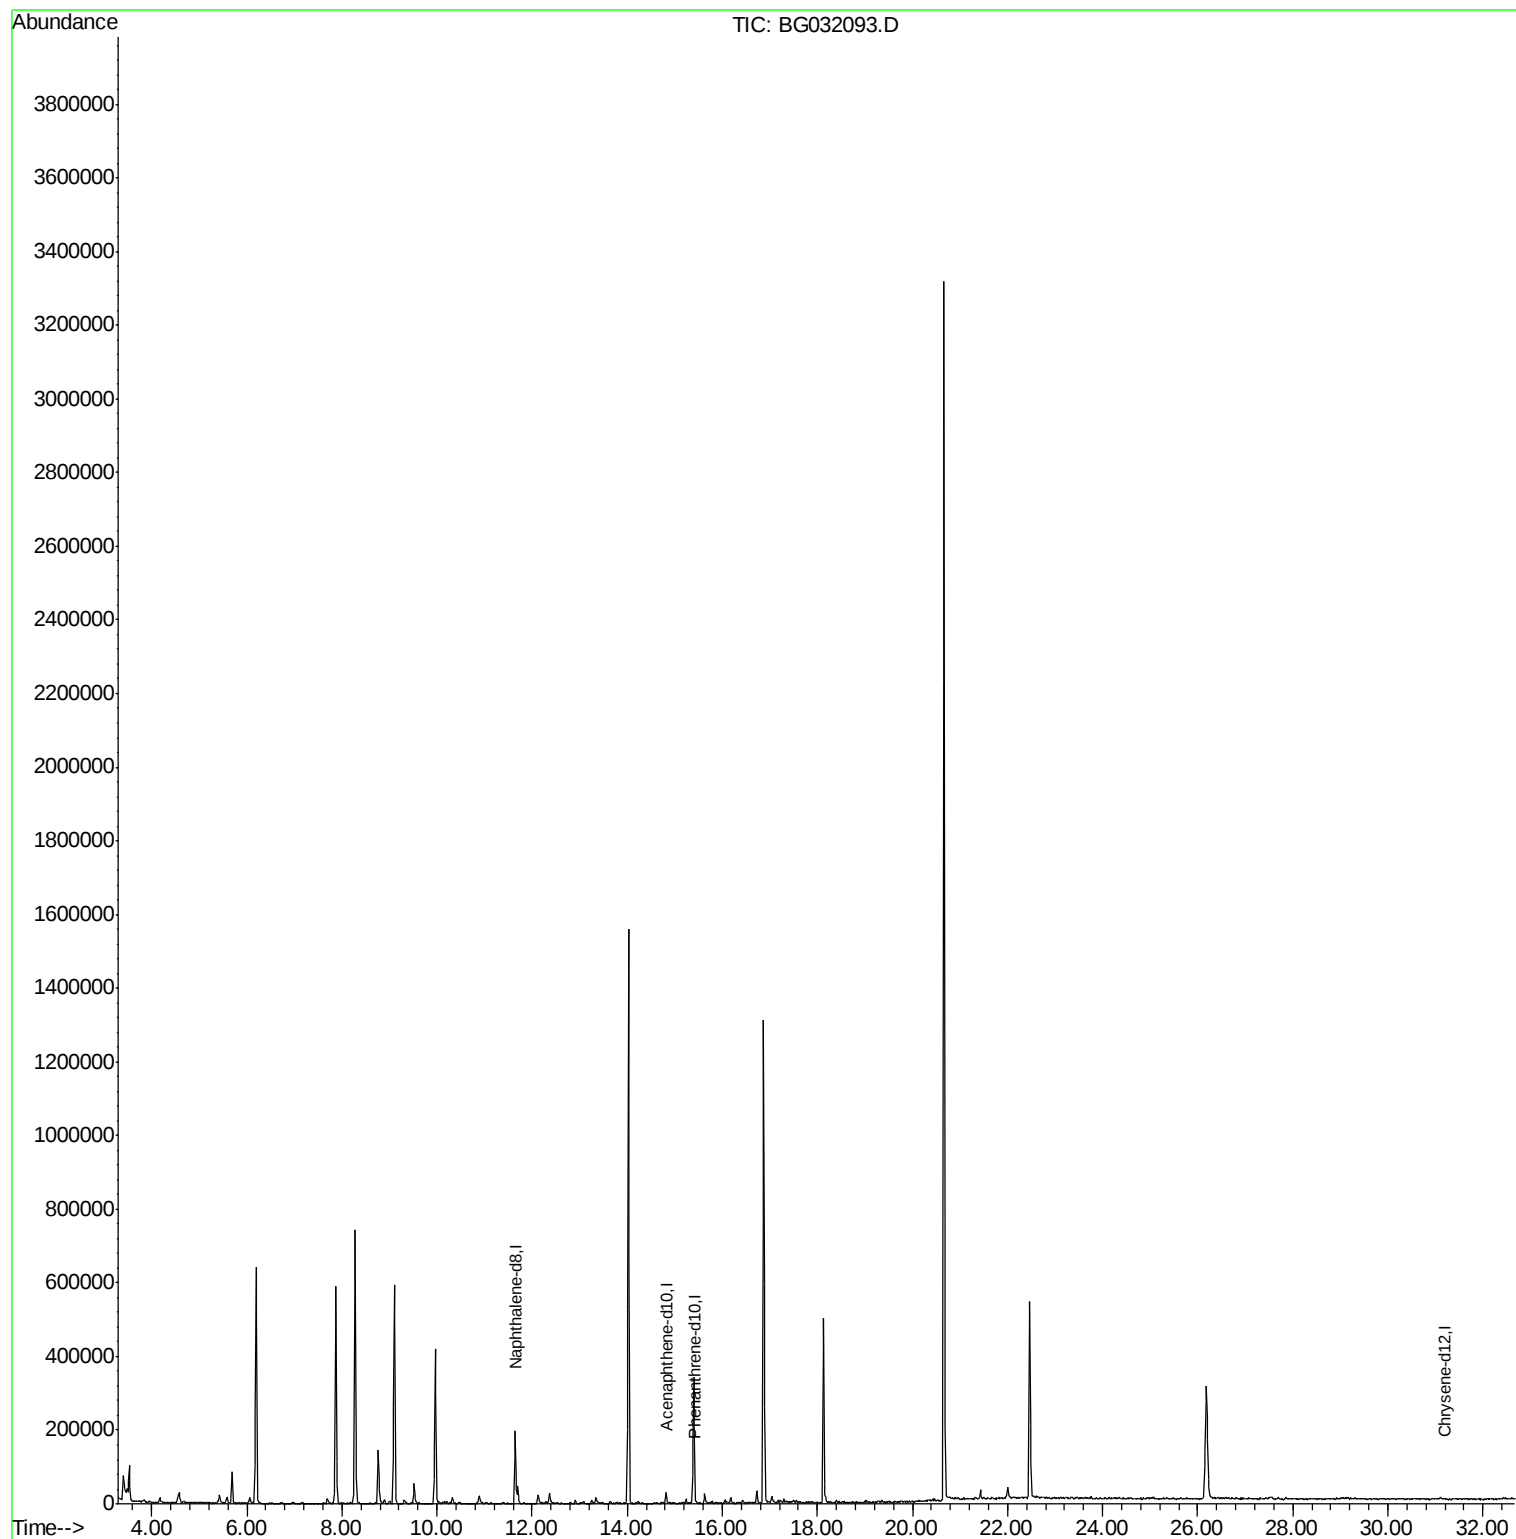


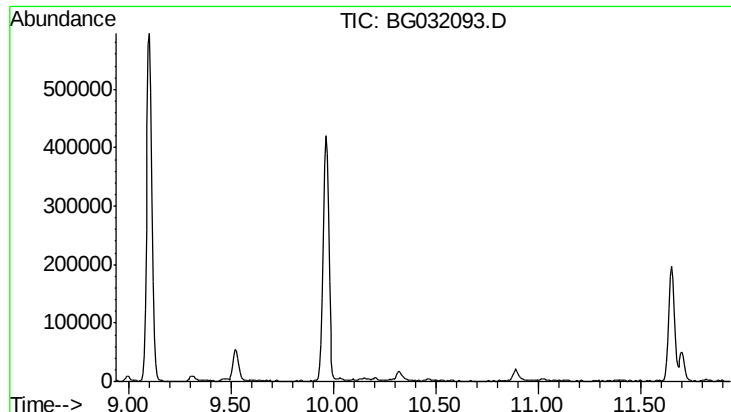

#5  
DDE  
Concen: N.D.  
Expected RT: 10.44 min  
Lab File: BG032093.D  
Acq: 17 Jan 2018 6:05


Instrument :  
BNA\_G  
ClientSampleId :


Tot Ion: 246  
Sig Exp Ratio  
246 100  
248 1793.6  
318 201.9  
176 4805.3

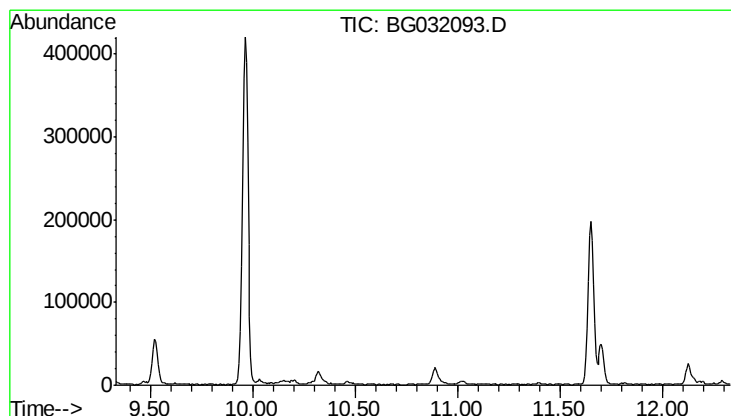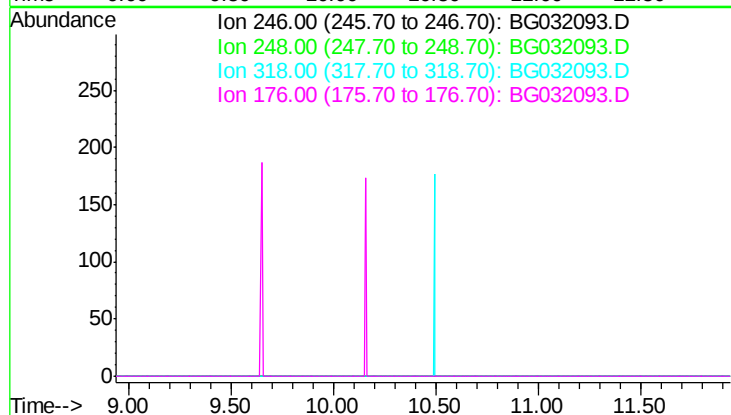

#6  
DDD  
Concen: N.D.  
Expected RT: 10.83 min  
Lab File: BG032093.D  
Acq: 17 Jan 2018 6:05

Tgt Ion: 235  
Sig Exp Ratio  
235 100  
237 6000.0  
165 6000.0

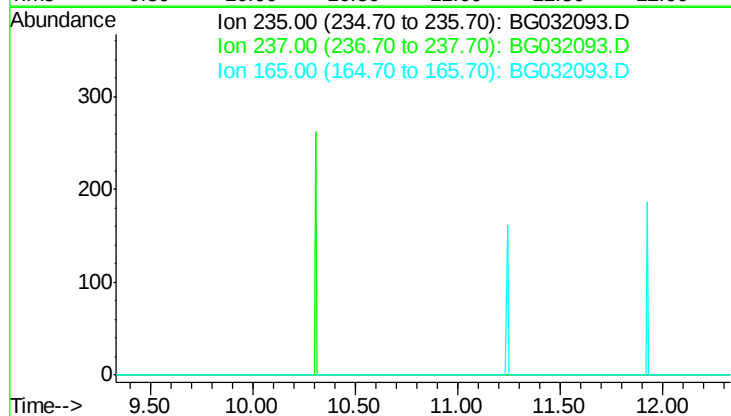

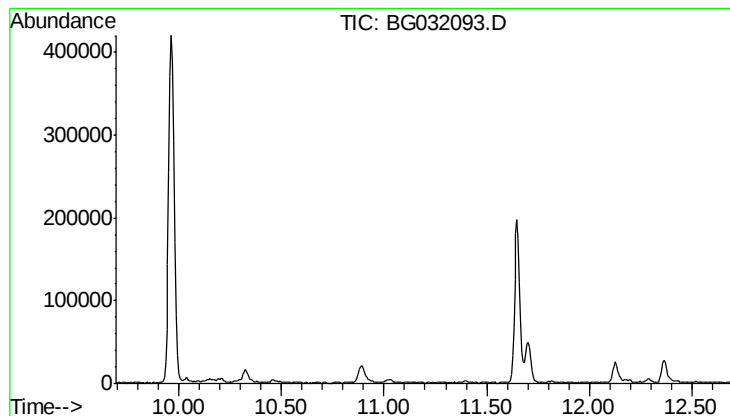

#7

DDT

Concen: N.D.

Expected RT: 11.19 min

Lab File: BG032093.D

Acq: 17 Jan 2018 6:05

Instrument :

BNA\_G

ClientSampleId :

Tot Ion: 235

Sig Exp Ratio

235 100

237 0.0

165 0.2

