

Data Path : U:\HPCHEM1\BNA G\DATA\BG011618\
 Data File : BG032094.D
 Acq On : 17 Jan 2018 6:42
 Operator : SJ/JU
 Sample : J1113-05
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Jan 17 08:07:07 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\BFDDTBREAKDOWN.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 01 16:14:27 2010
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	0.00	152	0	0.00	ng	-10.26
2) Naphthalene-d8	11.65	136	191377	40.00	ng	-0.07
3) Acenaphthene-d10	14.82	164	7512	40.00	ng	-0.09
4) Phenanthrene-d10	0.00	188	0	0.00	ng	-15.09
8) Chrysene-d12	30.70	240	69	40.00	ng	-0.23
9) Perylene-d12	0.00	264	0	0.00	ng	-34.56
Target Compounds						Ovalue
5) DDE	10.90	246	59	N.D.		
6) DDD	0.00	235	0	N.D.		
7) DDT	0.00	235	0	N.D.		




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : U:\HPCHEM1\BNA G\DATA\BG011618\
Data File : BG032094.D
Acq On : 17 Jan 2018 6:42
Operator : SJ/JU
Sample : J1113-05
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Jan 17 08:07:07 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\BFDDTBREAKDOWN.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 01 16:14:27 2010
Response via : Initial Calibration

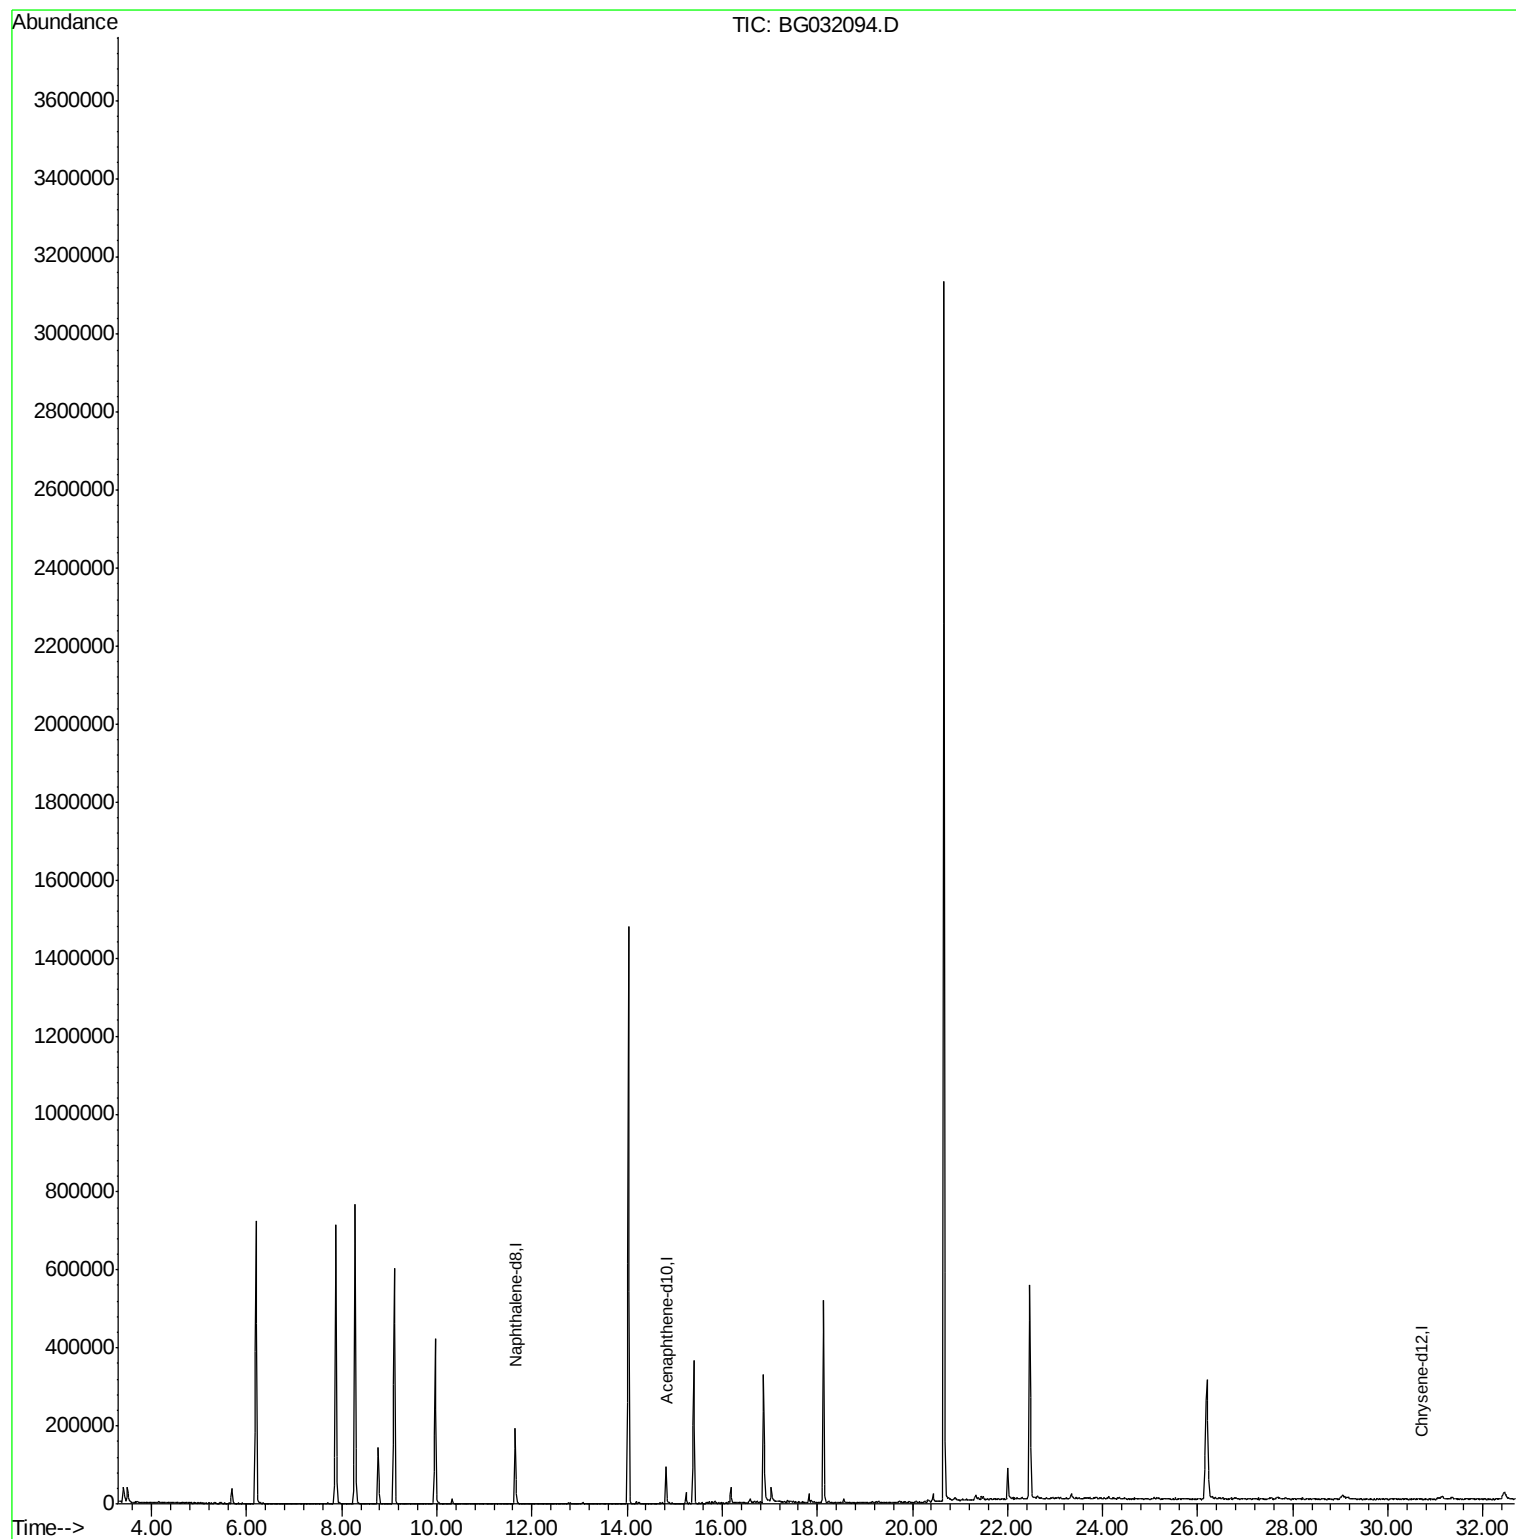

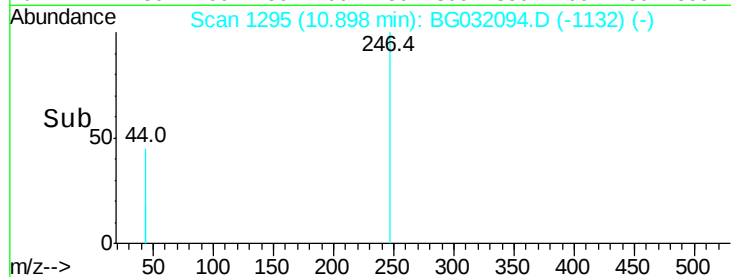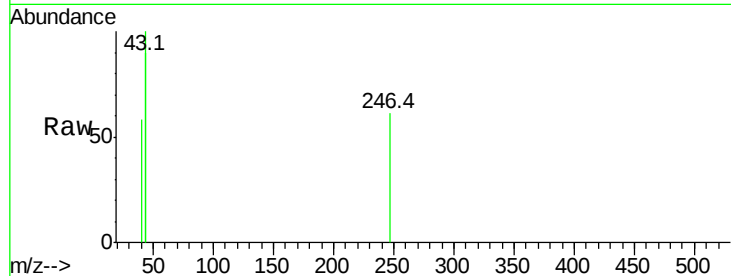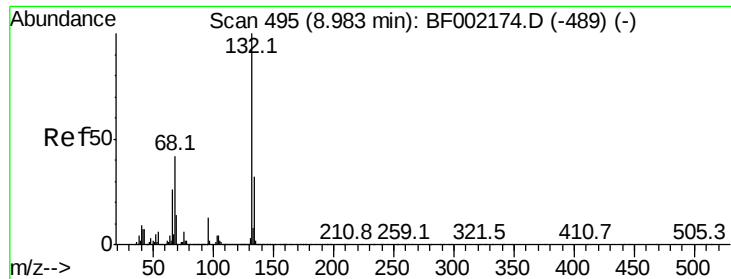

#5

DDE

Concen: N.D.

RT: 10.90 min Scan# 1295

Delta R.T. 0.46 min

Lab File: BG032094.D

Acq: 17 Jan 2018 6:42

Instrument :

BNA_G

ClientSampleId :

Tot Ion:246 Resp: 59



Ion Ratio Lower Upper

246 100

248 0.0 1434.9 2152.3#

318 91.5 161.5 242.3#

176 0.0 3844.2 5766.4#

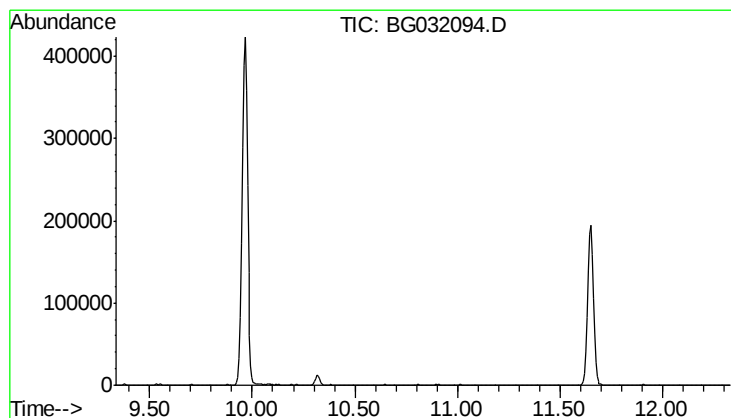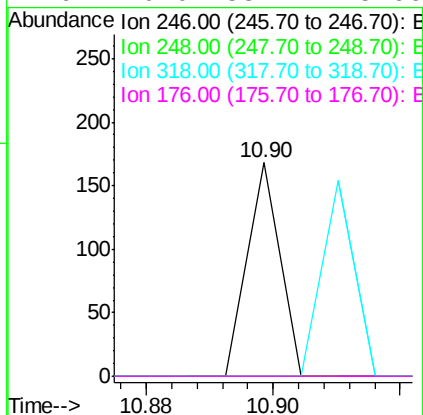

#6

DDD

Concen: N.D.

Expected RT: 10.83 min

Lab File: BG032094.D

Acq: 17 Jan 2018 6:42


Tgt Ion: 235


Sig Exp Ratio

235 100

237 6000.0

165 6000.0

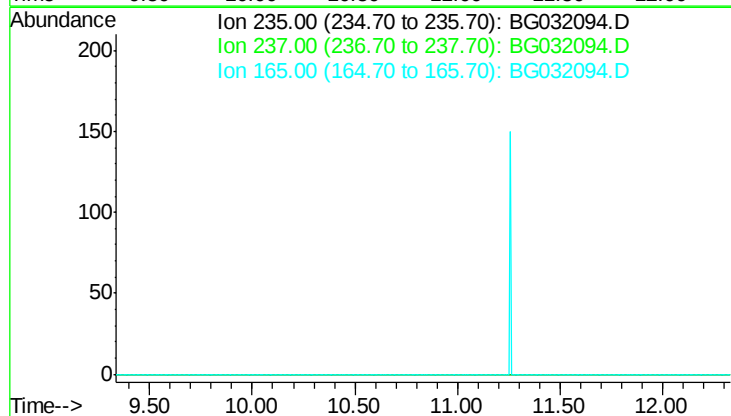

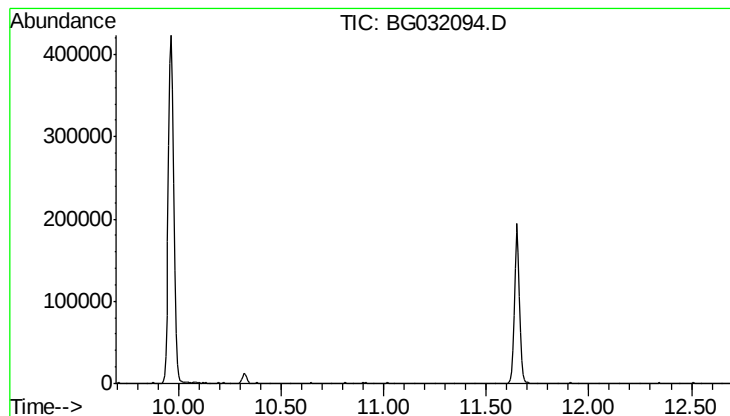

#7

DDT

Concen: N.D.

Expected RT: 11.19 min

Lab File: BG032094.D

Acq: 17 Jan 2018 6:42

Instrument :

BNA_G

ClientSampleId :

Tot Ion: 235

Sig Exp Ratio

235 100

237 0.0

165 0.2

