
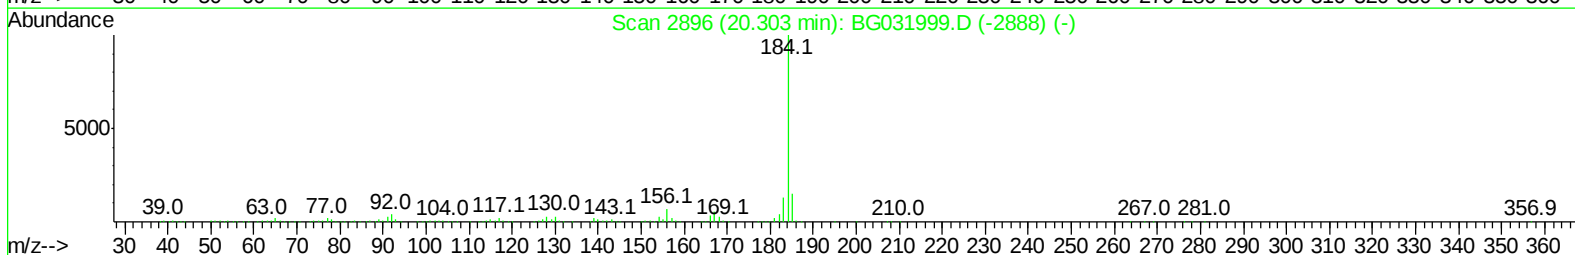
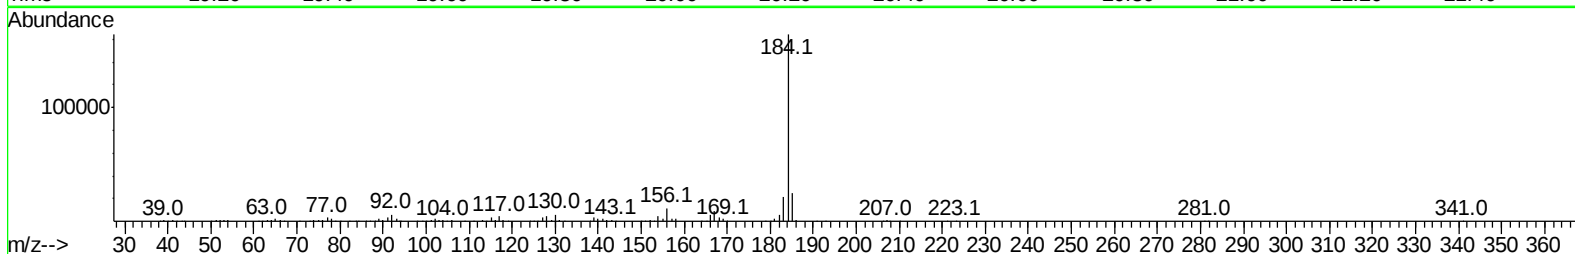


Data Path : U:\HPCHEM1\BNA G\DATA\BG011618\
Data File : BG032069.D
Acq On : 16 Jan 2018 14:52
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 17 07:26:33 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG011218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 15 10:05:15 2018
Response via : Initial Calibration

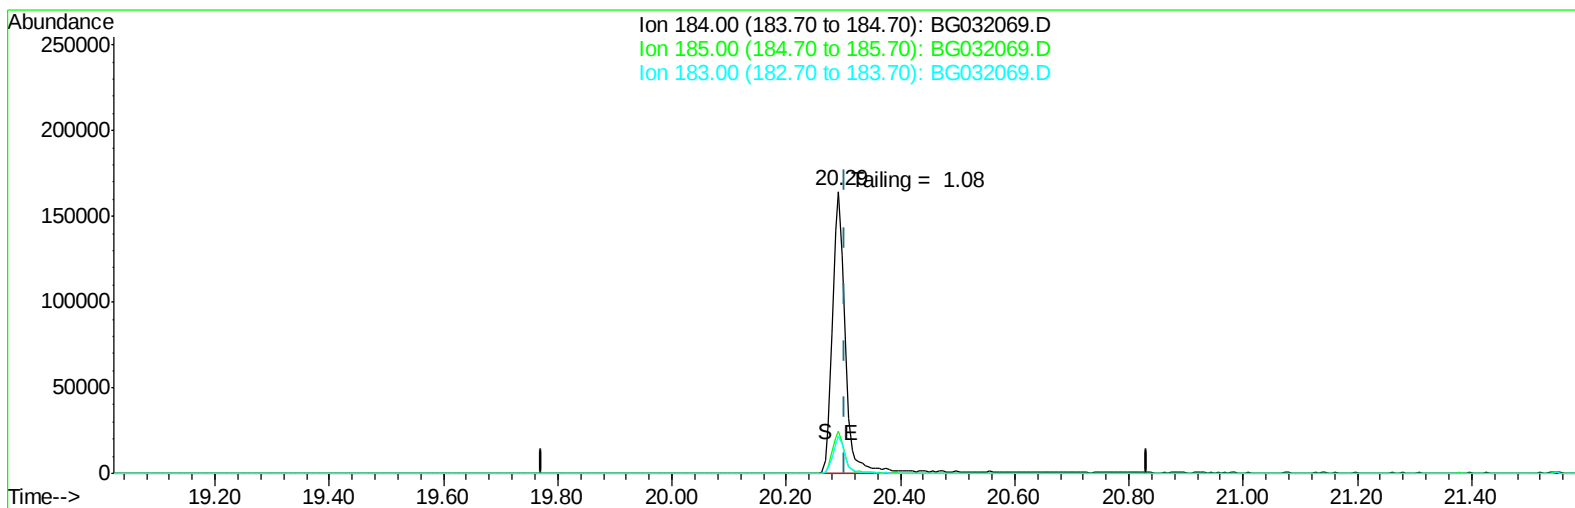

TIC: BG032069.D

(76) Benzidine




20.292min (-0.011) 0.00ng

response 251284

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	15.03
183.00	13.30	13.02
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA G\DATA\BG011618\
Data File : BG032069.D
Acq On : 16 Jan 2018 14:52
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 17 07:26:33 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG011218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 15 10:05:15 2018
Response via : Initial Calibration

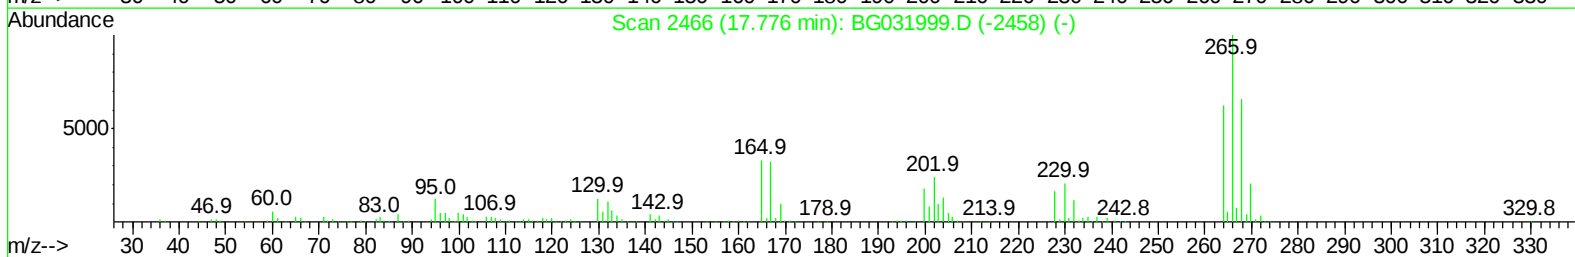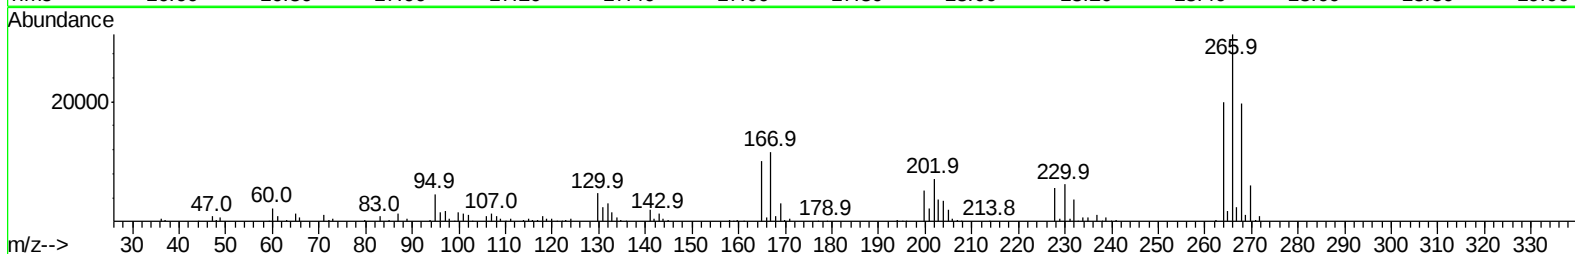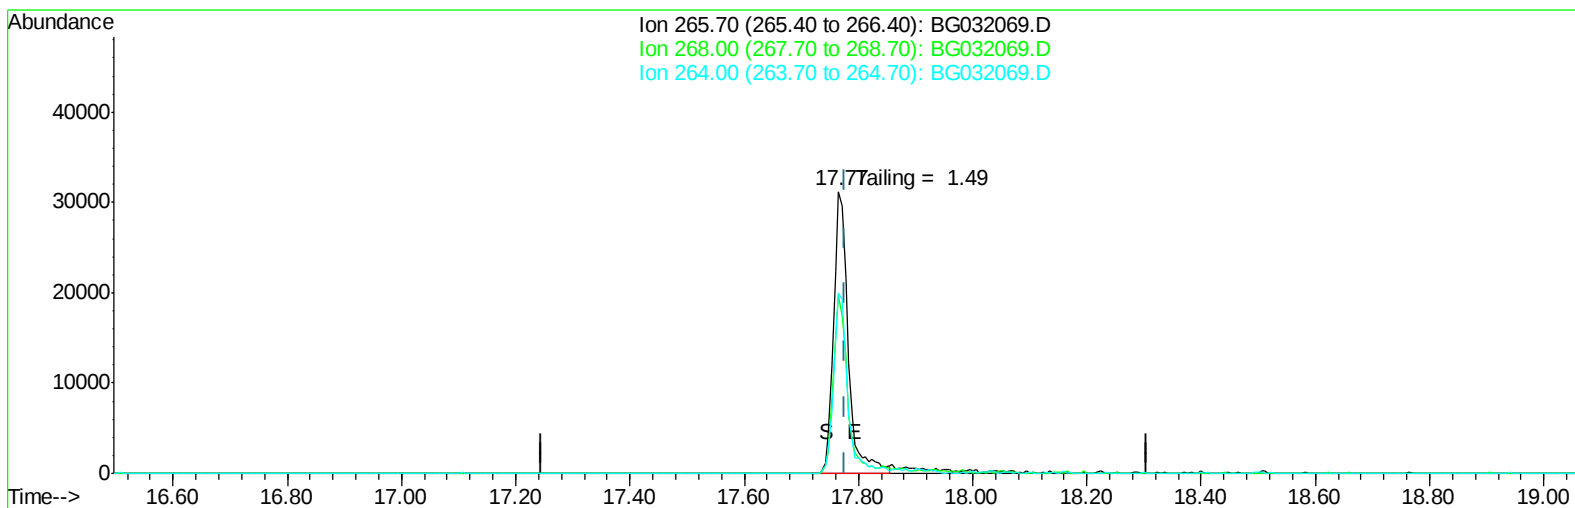

TIC: BG032069.D

(69) Pentachlorophenol (C)

17.765min (-0.011) 19473.65ng

response 55254

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.25
264.00	62.00	63.95
0.00	0.00	0.00