
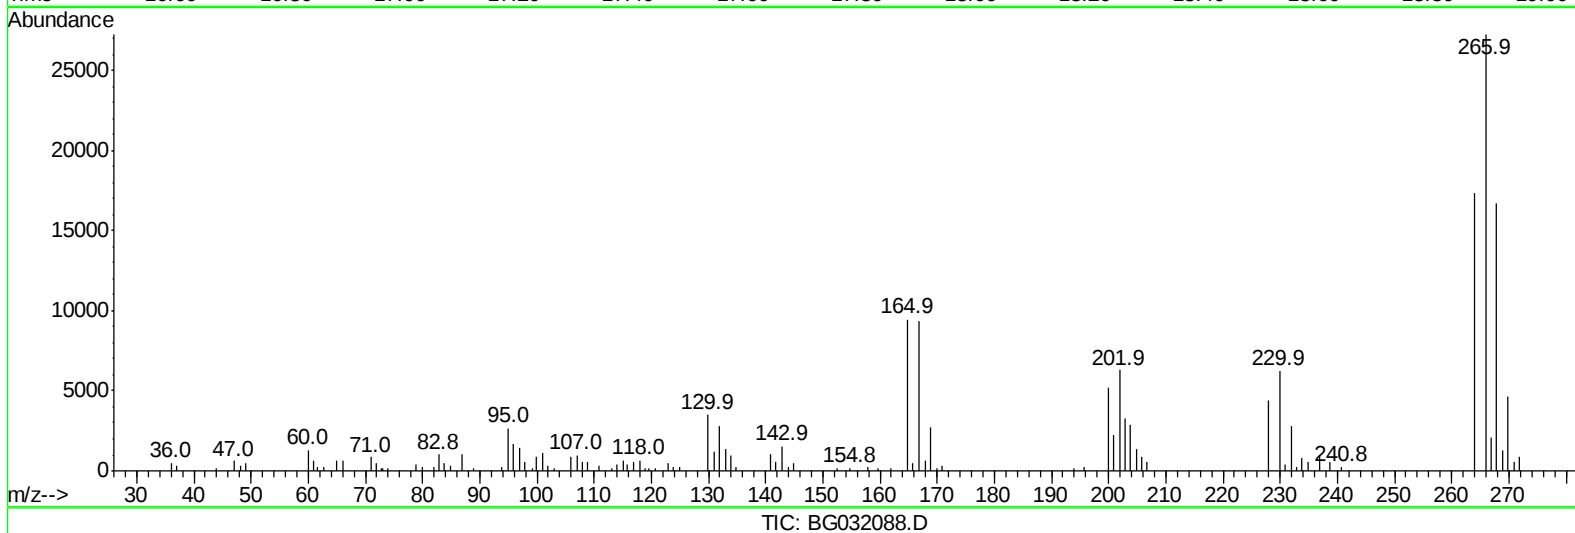


Data Path : U:\HPCHEM1\BNA G\DATA\BG011618\
Data File : BG032088.D
Acq On : 17 Jan 2018 2:45
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 17 07:27:55 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG011218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 15 10:05:15 2018
Response via : Initial Calibration

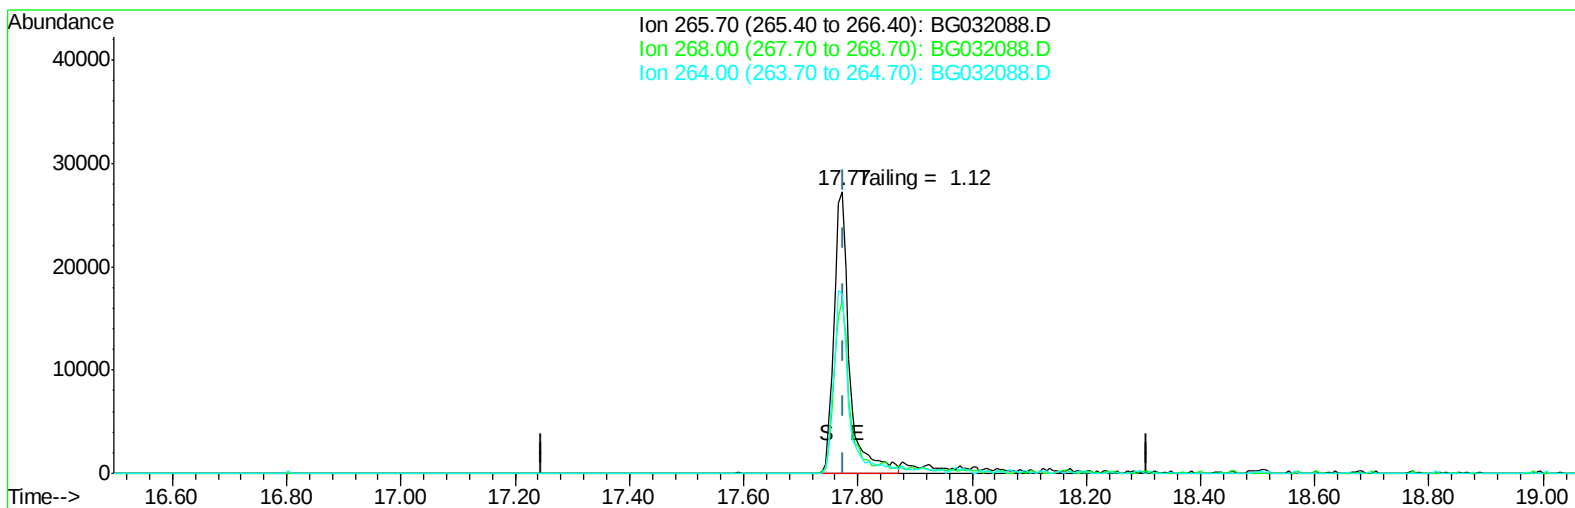

(69) Pentachlorophenol (C)



17.772min (-0.004) 14173.41ng

response 51196

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	61.33
264.00	62.00	63.71
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA G\DATA\BG011618\
Data File : BG032088.D
Acq On : 17 Jan 2018 2:45
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 17 07:27:55 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG011218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 15 10:05:15 2018
Response via : Initial Calibration

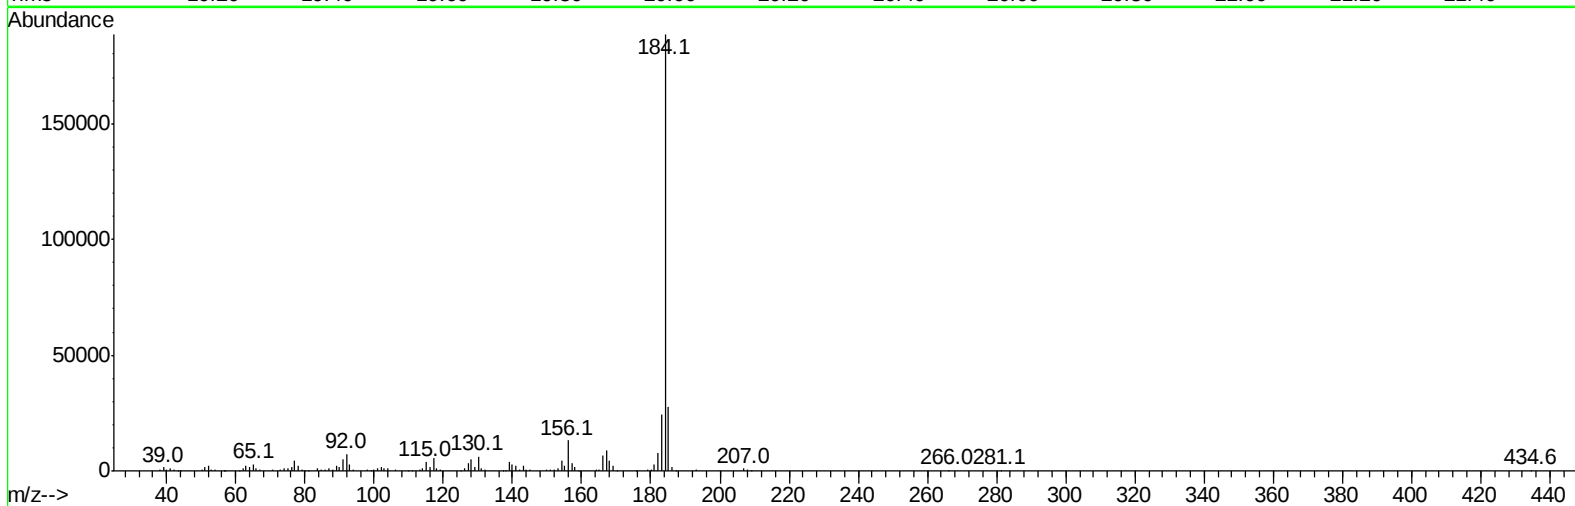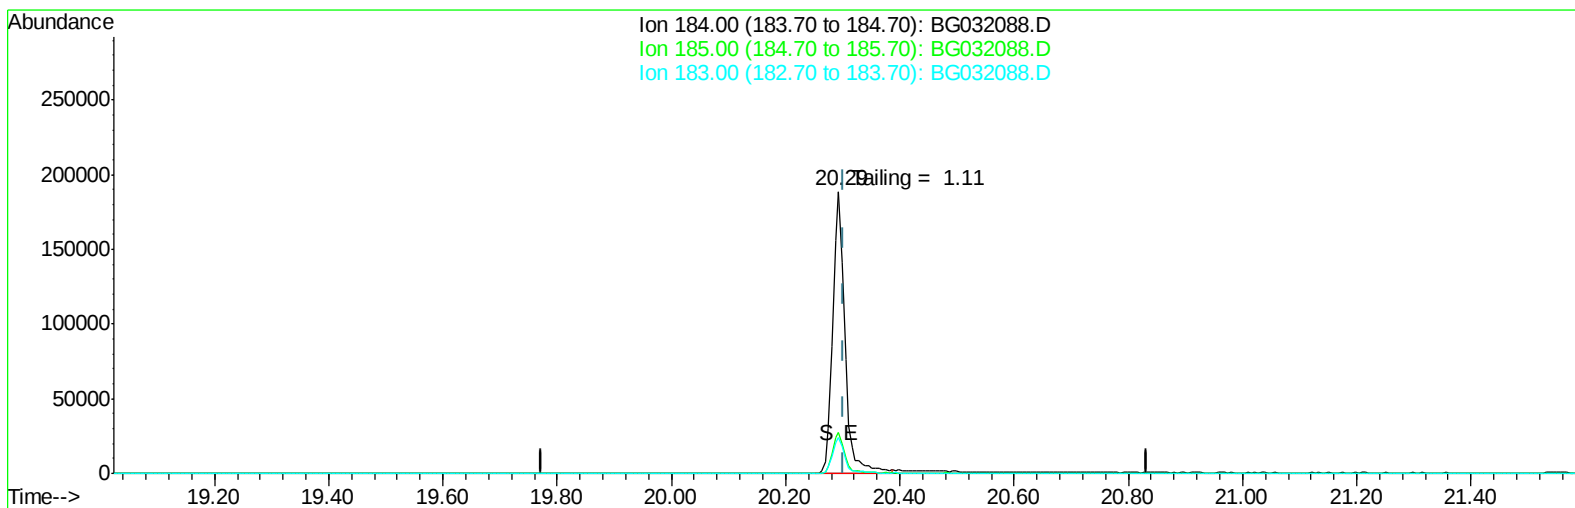

TIC: BG032088.D

(76) Benzidine

20.293min (-0.010) 0.00ng

response 281730

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.73
183.00	13.30	12.80
0.00	0.00	0.00