


Data Path : Z:\HPCHEM1\BNA_G\Data\BG011618\
 Data File : BG032069.D
 Acq On : 16 Jan 2018 14:52
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG011218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 15 10:05:15 2018

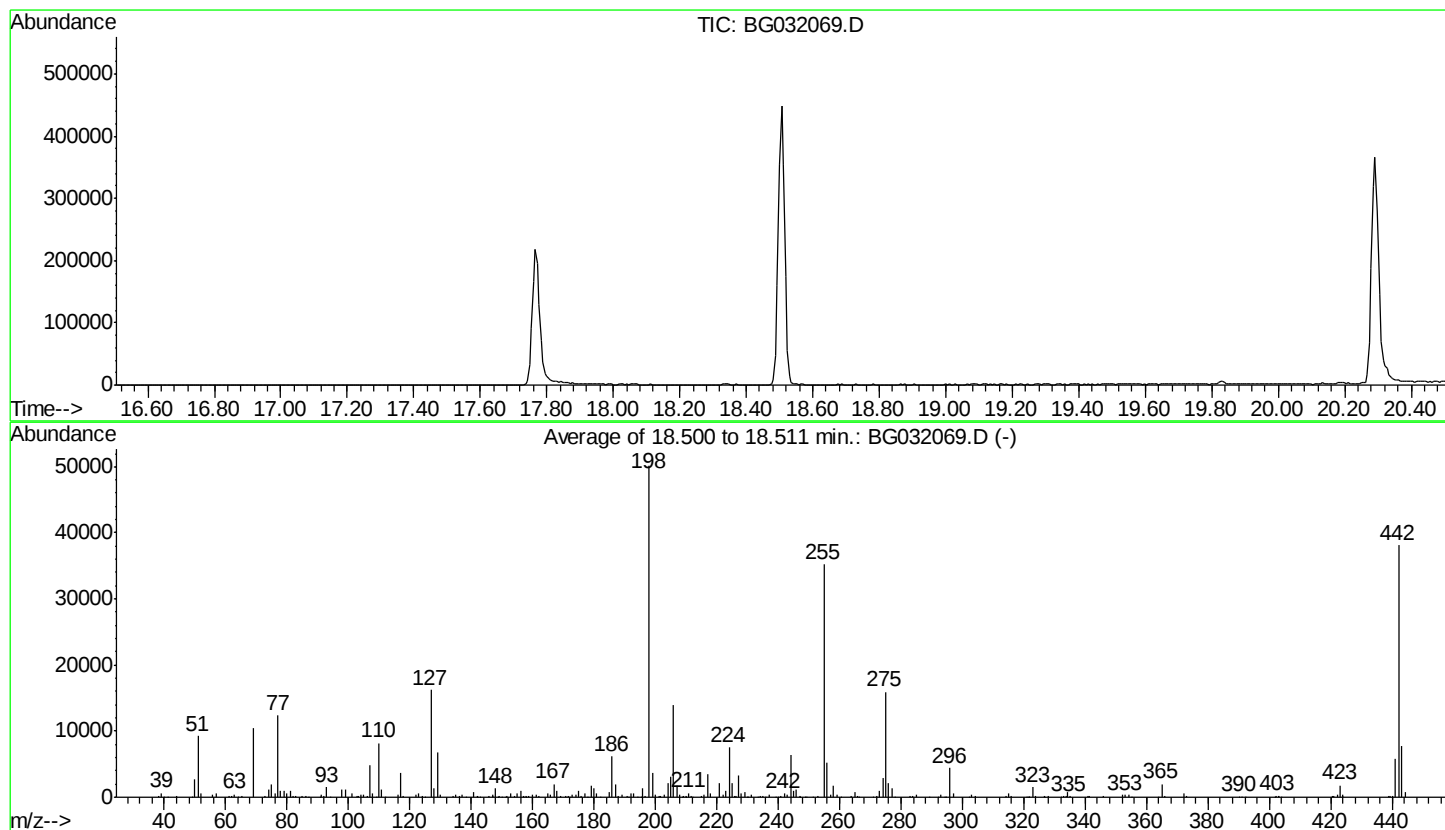

AutoFind: Scans 2589, 2590, 2591; Background Corrected with Scan 2582

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	18.4	9242	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	20.8	10438	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	32.3	16193	PASS
197	198	0.00	2	0.4	177	PASS
198	198	100	100	100.0	50165	PASS
199	198	5	9	7.4	3692	PASS
275	198	10	60	31.8	15969	PASS
365	198	1	100	3.9	1950	PASS
441	442	0.01	24	15.3	5842	PASS
442	198	50	100	75.9	38072	PASS
443	442	15	24	20.5	7809	PASS