


Data Path : Z:\HPCHEM1\BNA_G\Data\BG011618\
 Data File : BG032088.D
 Acq On : 17 Jan 2018 2:45
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG011218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 15 10:05:15 2018

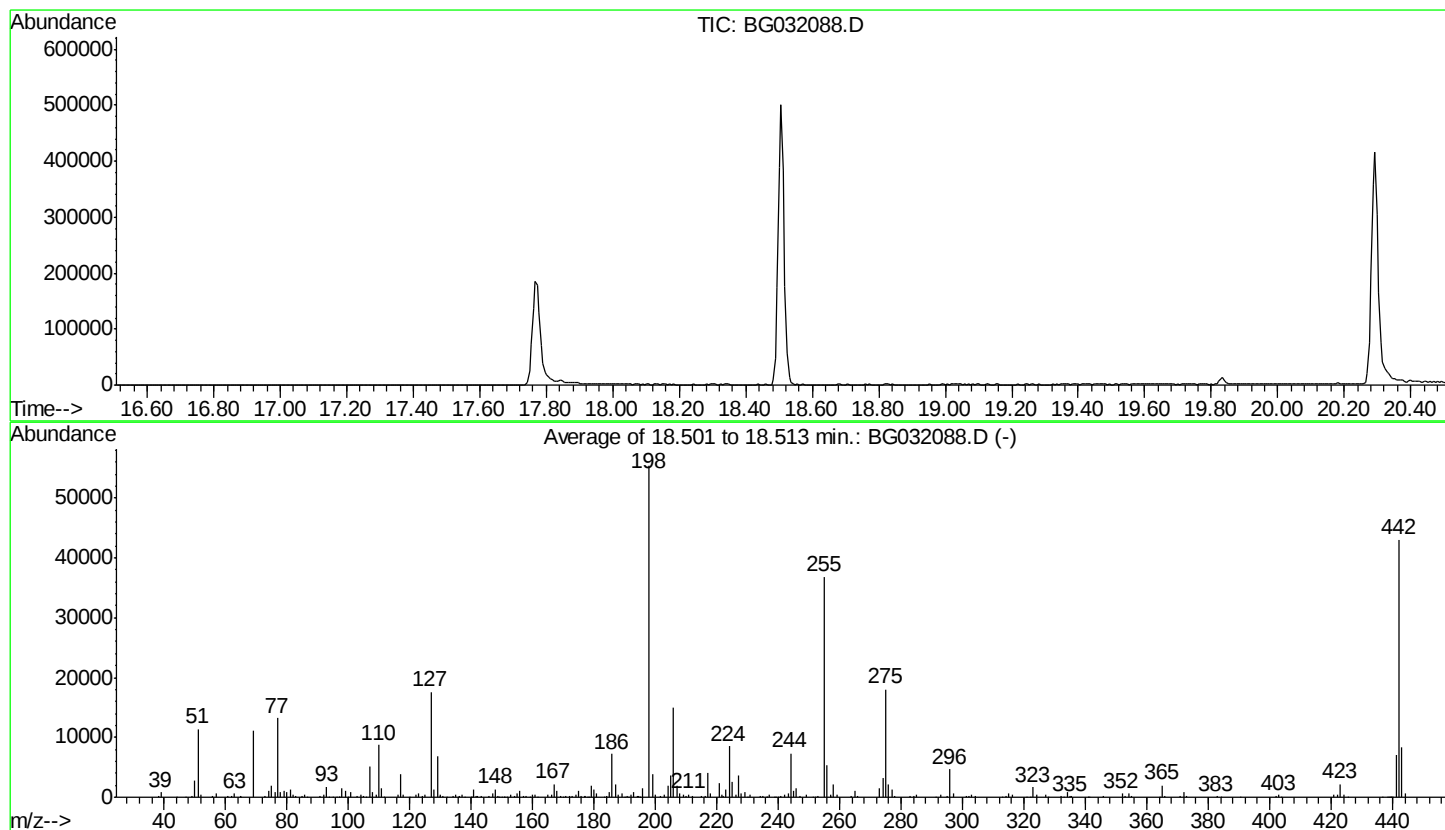

AutoFind: Scans 2589, 2590, 2591; Background Corrected with Scan 2583

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	20.5	11370	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	20.3	11226	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	31.8	17628	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	55413	PASS
199	198	5	9	6.9	3802	PASS
275	198	10	60	32.6	18078	PASS
365	198	1	100	3.5	1946	PASS
441	442	0.01	24	16.3	7000	PASS
442	198	50	100	77.7	43032	PASS
443	442	15	24	19.6	8446	PASS