
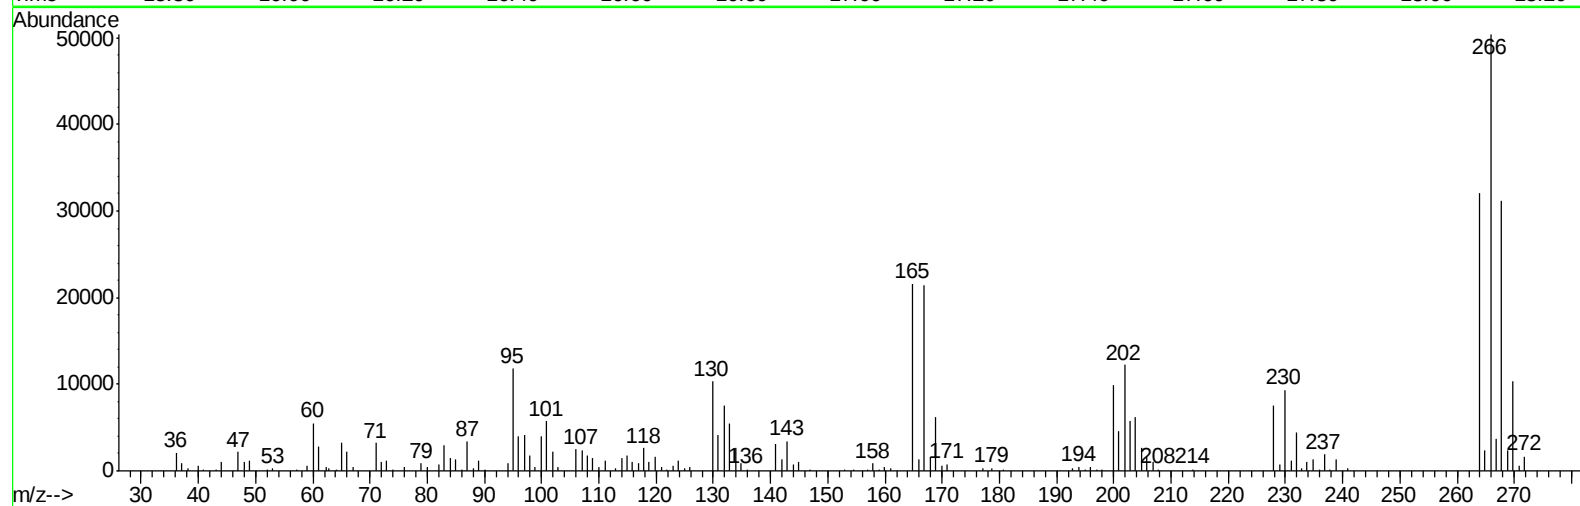


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG011620\
Data File : BG044061.D
Acq On : 16 Jan 2020 9:51
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 17 07:34:34 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG123019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 31 13:32:23 2019
Response via : Initial Calibration

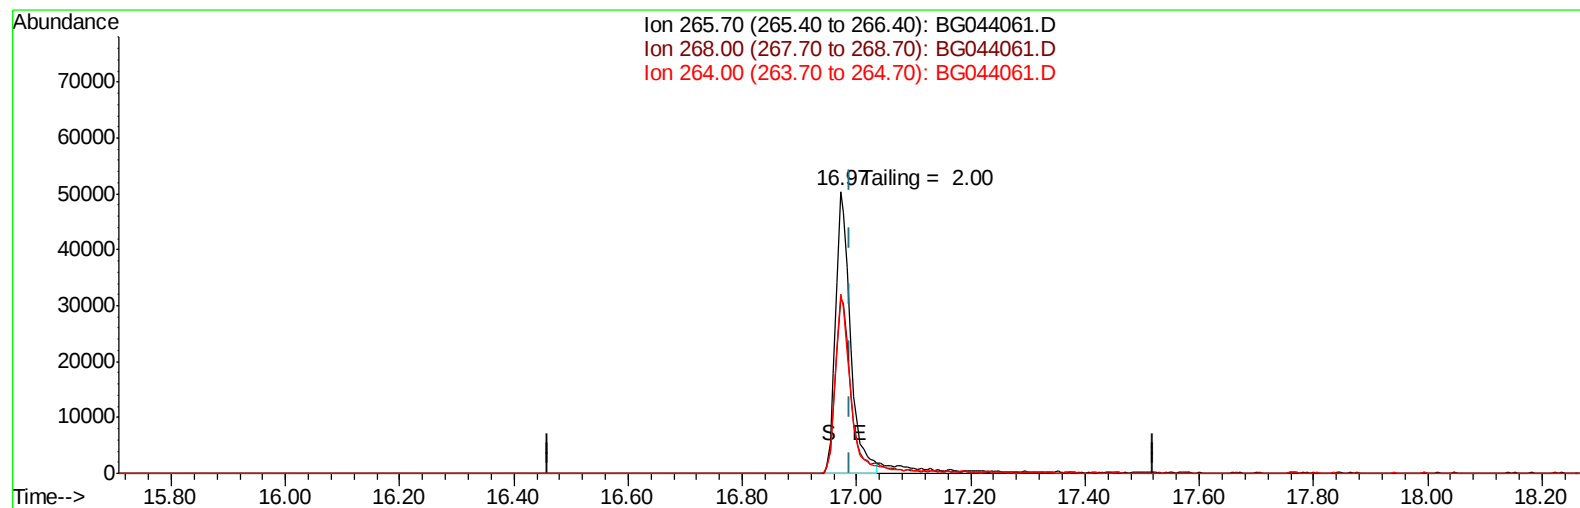

TIC: BG044061.D

(70) Pentachlorophenol (C)



16.971min (-0.018) 26100.91ng

response 93113

Ion	Exp%	Act%
265.70	100	100
268.00	65.80	61.88
264.00	63.50	63.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG011620\
 Data File : BG044061.D
 Acq On : 16 Jan 2020 9:51
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 17 07:34:34 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG123019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 31 13:32:23 2019
 Response via : Initial Calibration

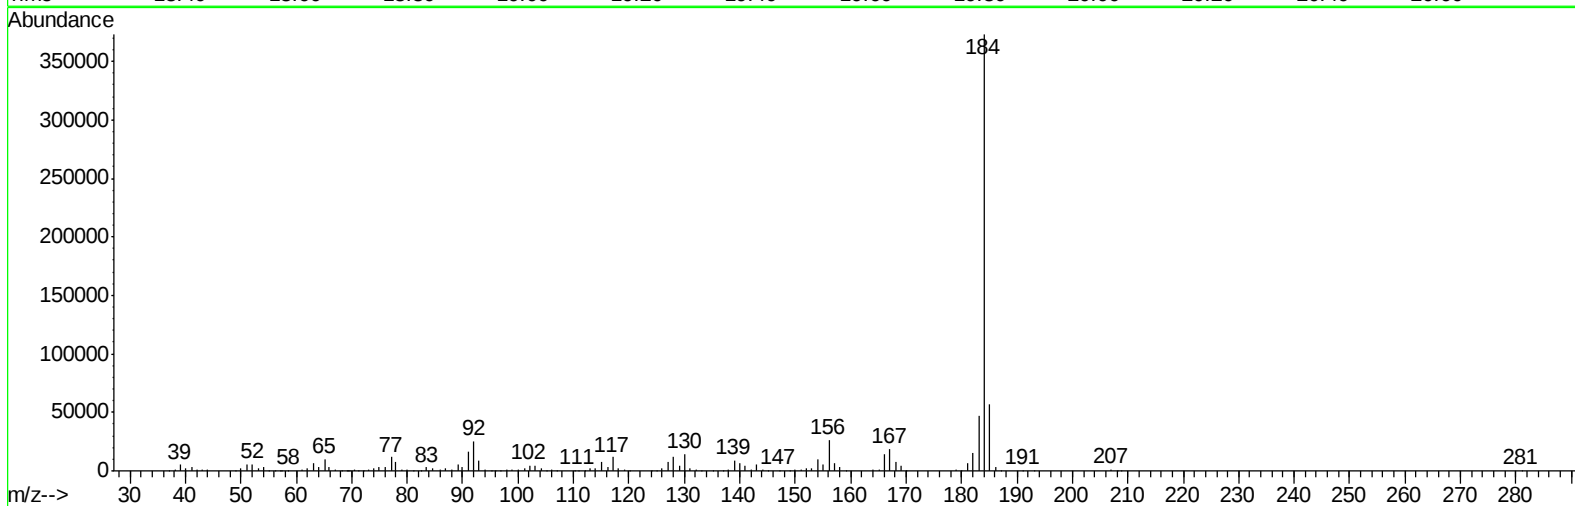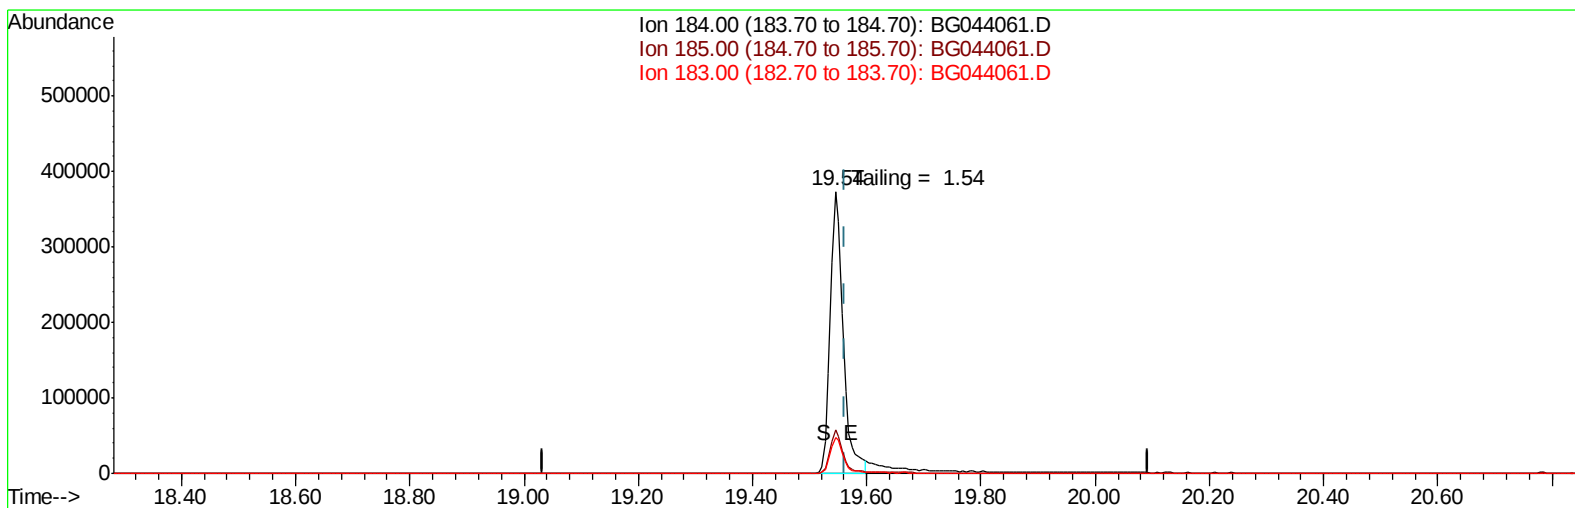

TIC: BG044061.D

(77) Benzidine

19.545min (-0.018) 0.00ng

response 632316

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	15.36
183.00	13.20	12.74
0.00	0.00	0.00