


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG011620\
 Data File : BG044061.D
 Acq On : 16 Jan 2020 9:51
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG123019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 31 13:32:23 2019

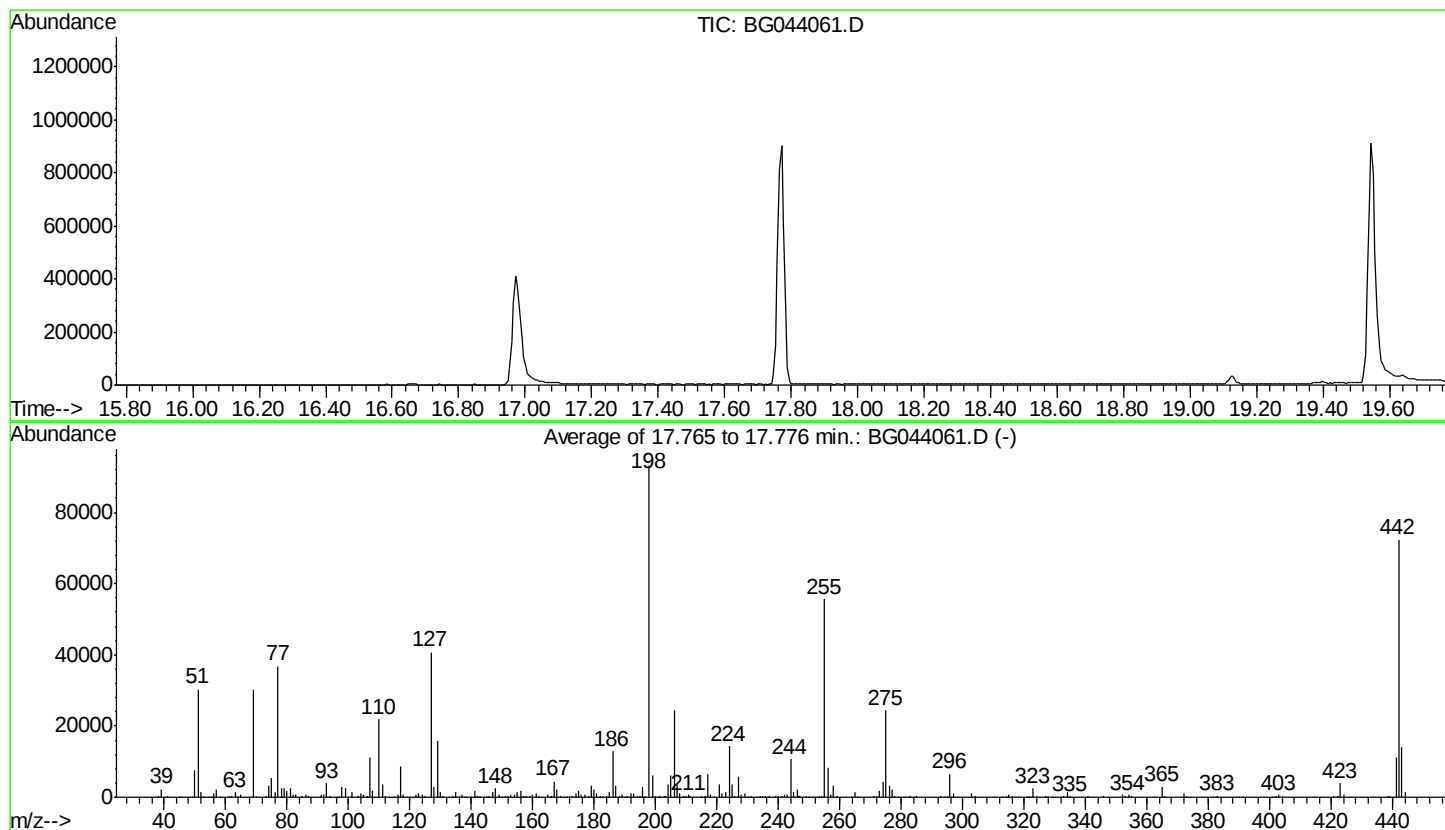

AutoFind: Scans 2498, 2499, 2500; Background Corrected with Scan 2491

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.6	30365	PASS
68	69	0.00	2	0.4	130	PASS
69	198	0.00	100	32.5	30285	PASS
70	69	0.00	2	0.2	70	PASS
127	198	10	80	43.7	40690	PASS
197	198	0.00	2	0.3	299	PASS
198	198	100	100	100.0	93149	PASS
199	198	5	9	6.6	6160	PASS
275	198	10	60	26.1	24309	PASS
365	198	1	100	3.2	2975	PASS
441	198	0.01	100	12.0	11210	PASS
442	198	50	100	77.7	72354	PASS
443	442	15	24	19.5	14123	PASS