
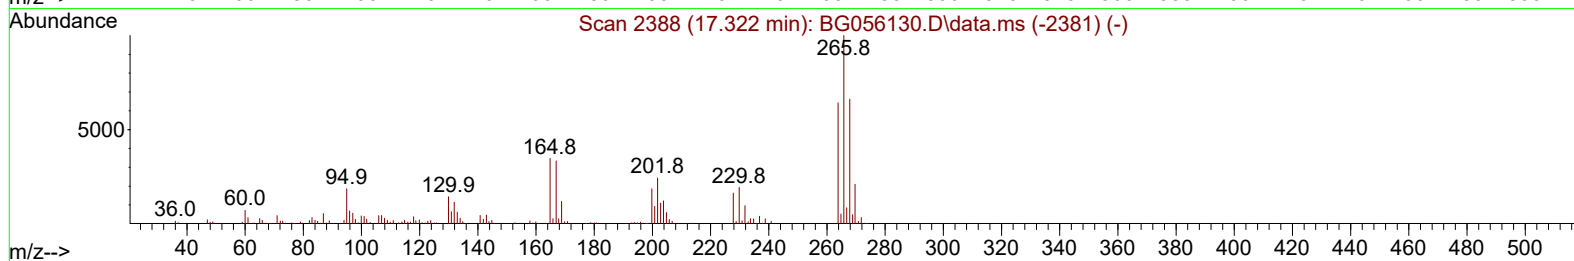
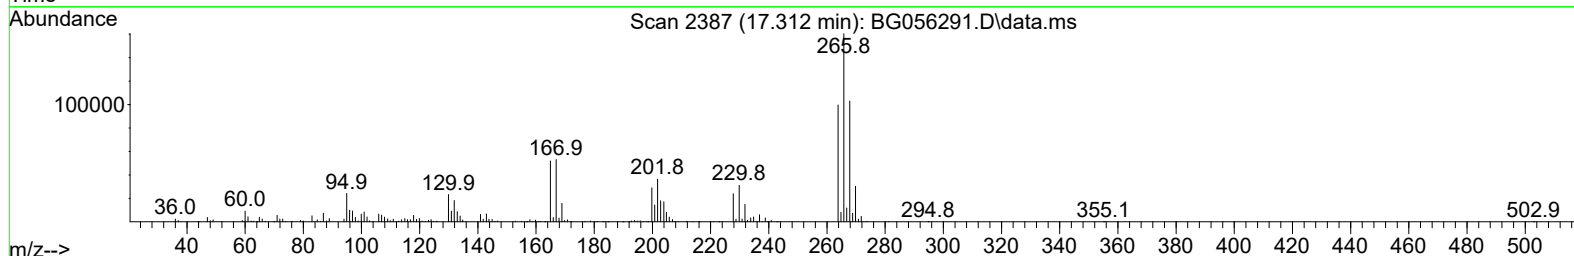


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011623\
Data File : BG056291.D
Acq On : 16 Jan 2023 10:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 17 07:48:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 12 03:38:40 2023
Response via : Initial Calibration

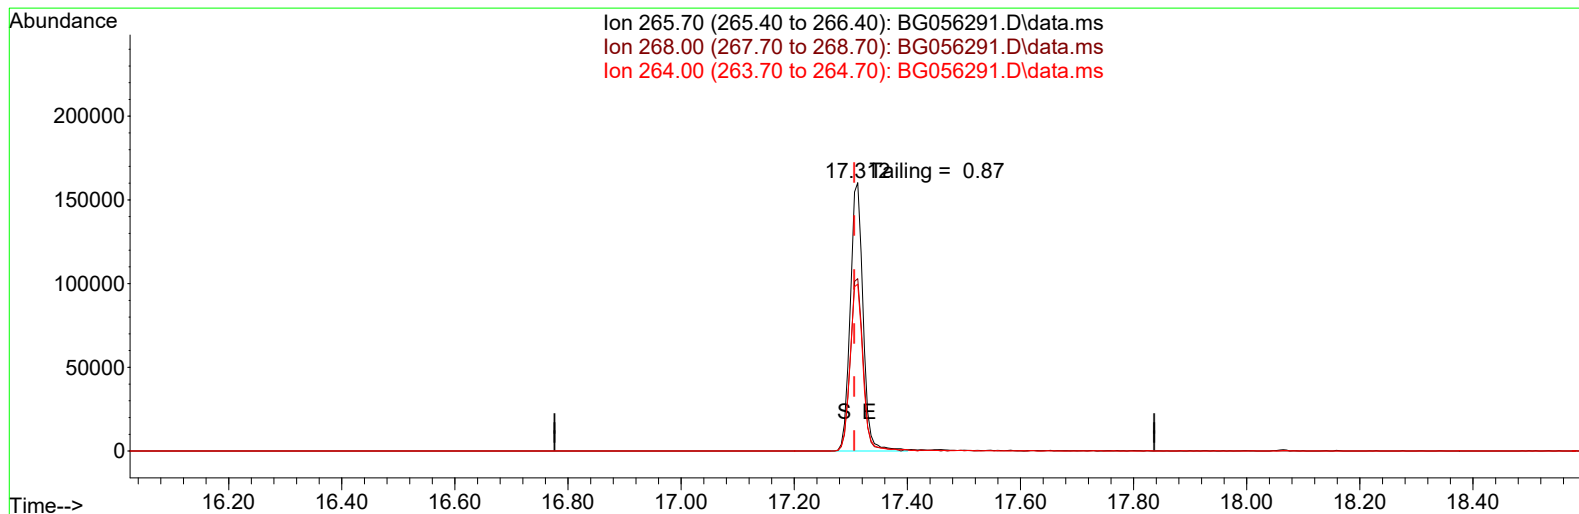

TIC: BG056291.D\data.ms

(70) Pentachlorophenol (C)




17.312min (+ 0.006) 306489.16 ng

response 254536

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.20	64.22
264.00	64.30	62.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011623\
 Data File : BG056291.D
 Acq On : 16 Jan 2023 10:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 17 07:48:41 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 12 03:38:40 2023
 Response via : Initial Calibration

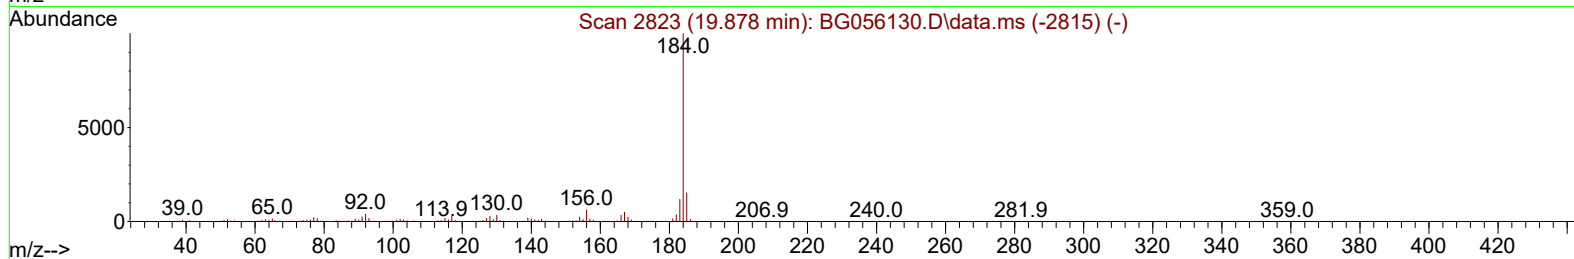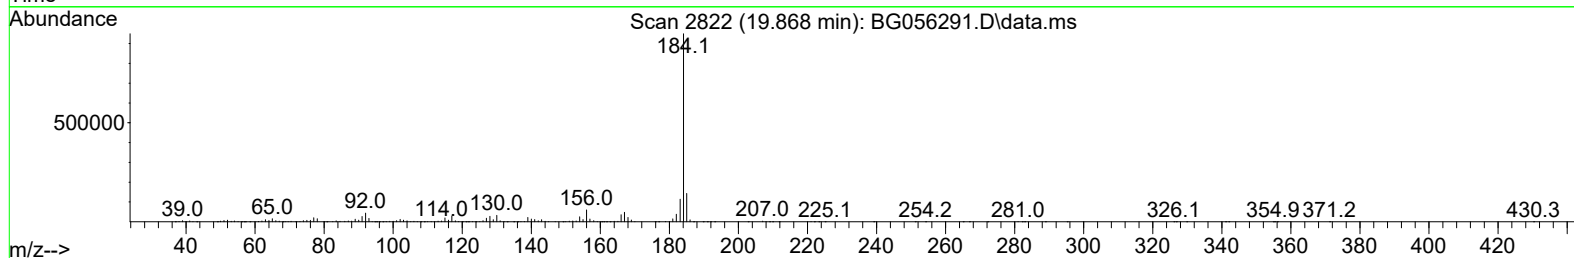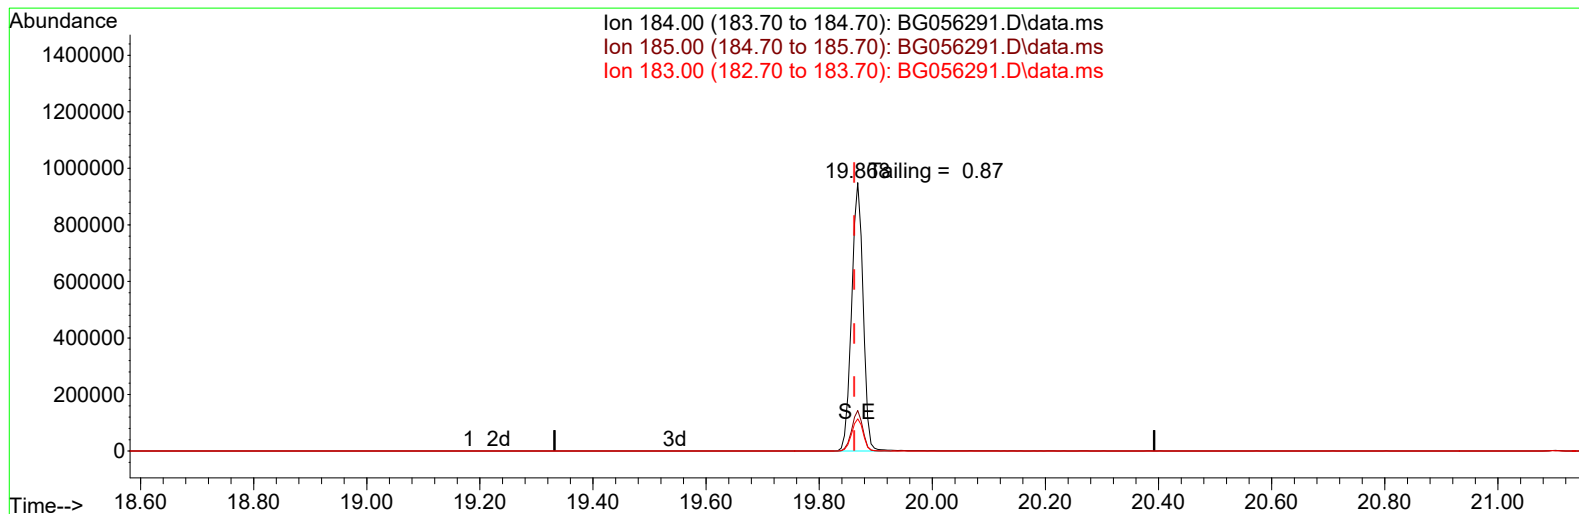

TIC: BG056291.D\data.ms

(77) Benzidine

19.868min (+ 0.006) 126234.37 ng m

response 1344834

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	15.09
183.00	11.70	11.98
0.00	0.00	0.00