

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011623\
 Data File : BG056293.D
 Acq On : 16 Jan 2023 12:26
 Operator : CG/JU
 Sample : PB150235BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB150235BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG056293.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.357	345	352	361	rBV	146996	234444	5.22%	1.556%
2	5.833	426	433	447	rVB	641710	1040012	23.16%	6.902%
3	7.448	699	708	717	rBV	632140	1093267	24.35%	7.255%
4	8.318	847	856	862	rBV	129353	221573	4.93%	1.470%
5	9.487	1047	1055	1066	rBV	364951	658045	14.65%	4.367%
6	11.150	1330	1338	1349	rBB	169165	303631	6.76%	2.015%
7	13.553	1740	1747	1759	rBV	1461218	2247055	50.04%	14.912%
8	14.928	1971	1981	1988	rBV	325368	526673	11.73%	3.495%
9	16.408	2225	2233	2246	rBV	1094032	1687479	37.58%	11.199%
10	17.660	2440	2446	2457	rBV	512111	775349	17.27%	5.146%
11	20.239	2879	2885	2891	rVB	3573261	4490501	100.00%	29.801%
12	21.955	3171	3177	3184	rVB	548470	889567	19.81%	5.904%
13	25.398	3753	3763	3775	rVB2	302269	900776	20.06%	5.978%




Sum of corrected areas: 15068372

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011623\
Data File : BG056293.D
Acq On : 16 Jan 2023 12:26
Operator : CG/JU
Sample : PB150235BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB150235BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

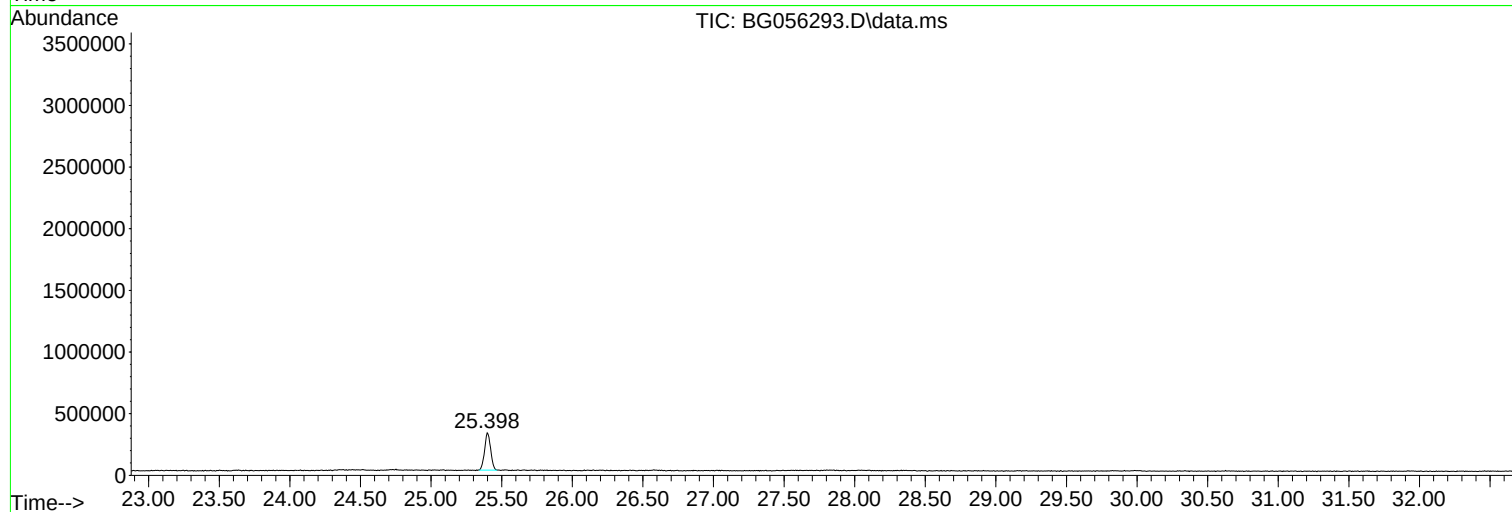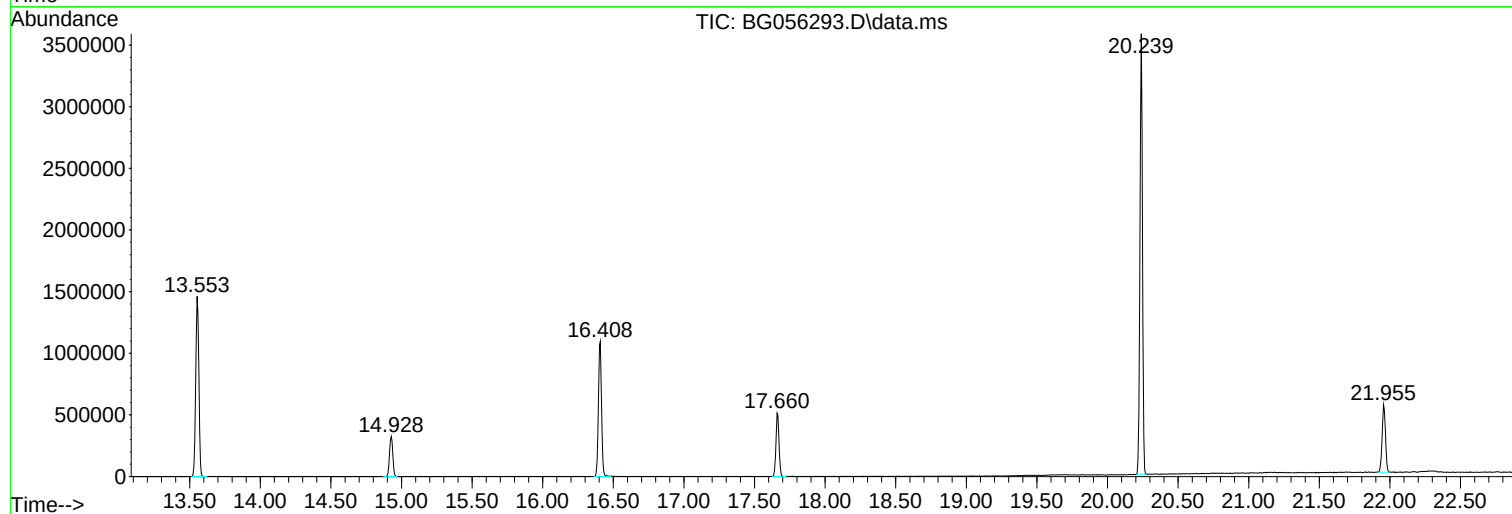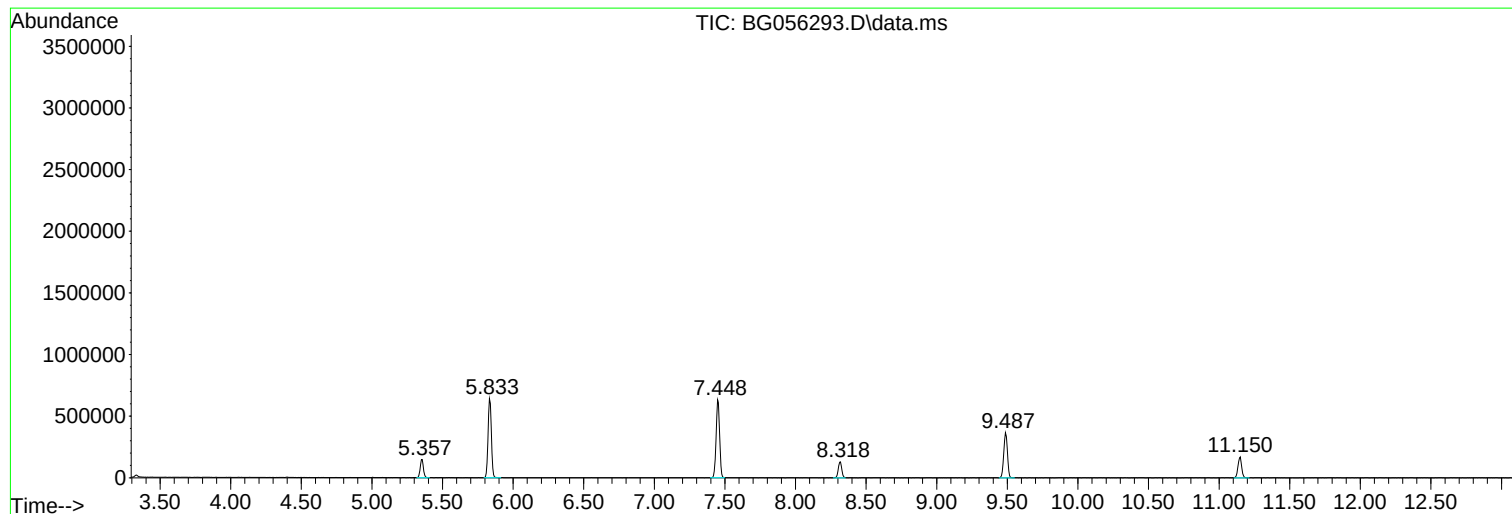

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011623\
Data File : BG056293.D
Acq On : 16 Jan 2023 12:26
Operator : CG/JU
Sample : PB150235BL
Misc :
ALS Vial : 3 Sample Multiplier: 1










Instrument :
BNA_G
ClientSampleId :
PB150235BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
5.357	21.16 ng	234444	1,4-Dichlorobenzene-d4	8.312	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56
2	Butanoic acid, 4-iodo-, methyl e...	228	C5H9IO2	014273-85-9	40
3	3-Hexanol, 4-ethyl-	130	C8H18O	019780-44-0	39
4	Butanoic acid, 4-(2-methoxy-1-me...	204	C9H16O5	054966-46-0	36
5	4-Ethyl-3-octanol	158	C10H22O	019781-26-1	25

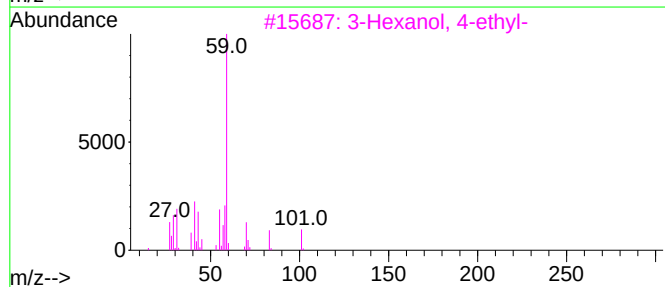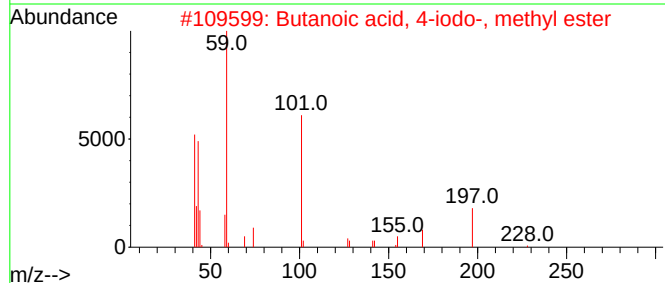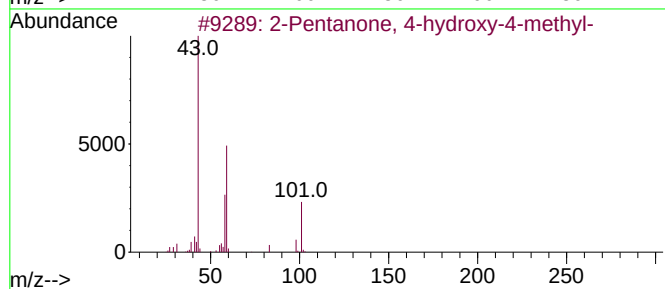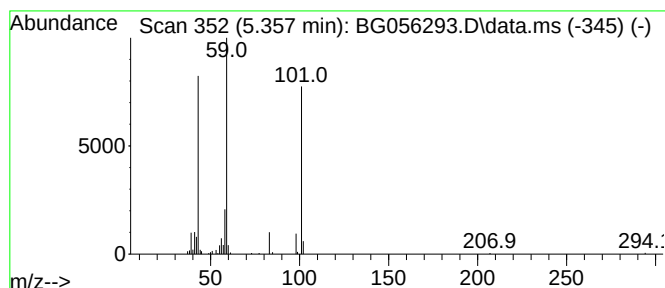

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011623\
Data File : BG056293.D
Acq On : 16 Jan 2023 12:26
Operator : CG/JU
Sample : PB150235BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB150235BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.357	21.2	ng	234444	1	8.312	221573	20.0