


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011623\
Data File : BG056291.D
Acq On : 16 Jan 2023 10:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jan 12 03:38:40 2023

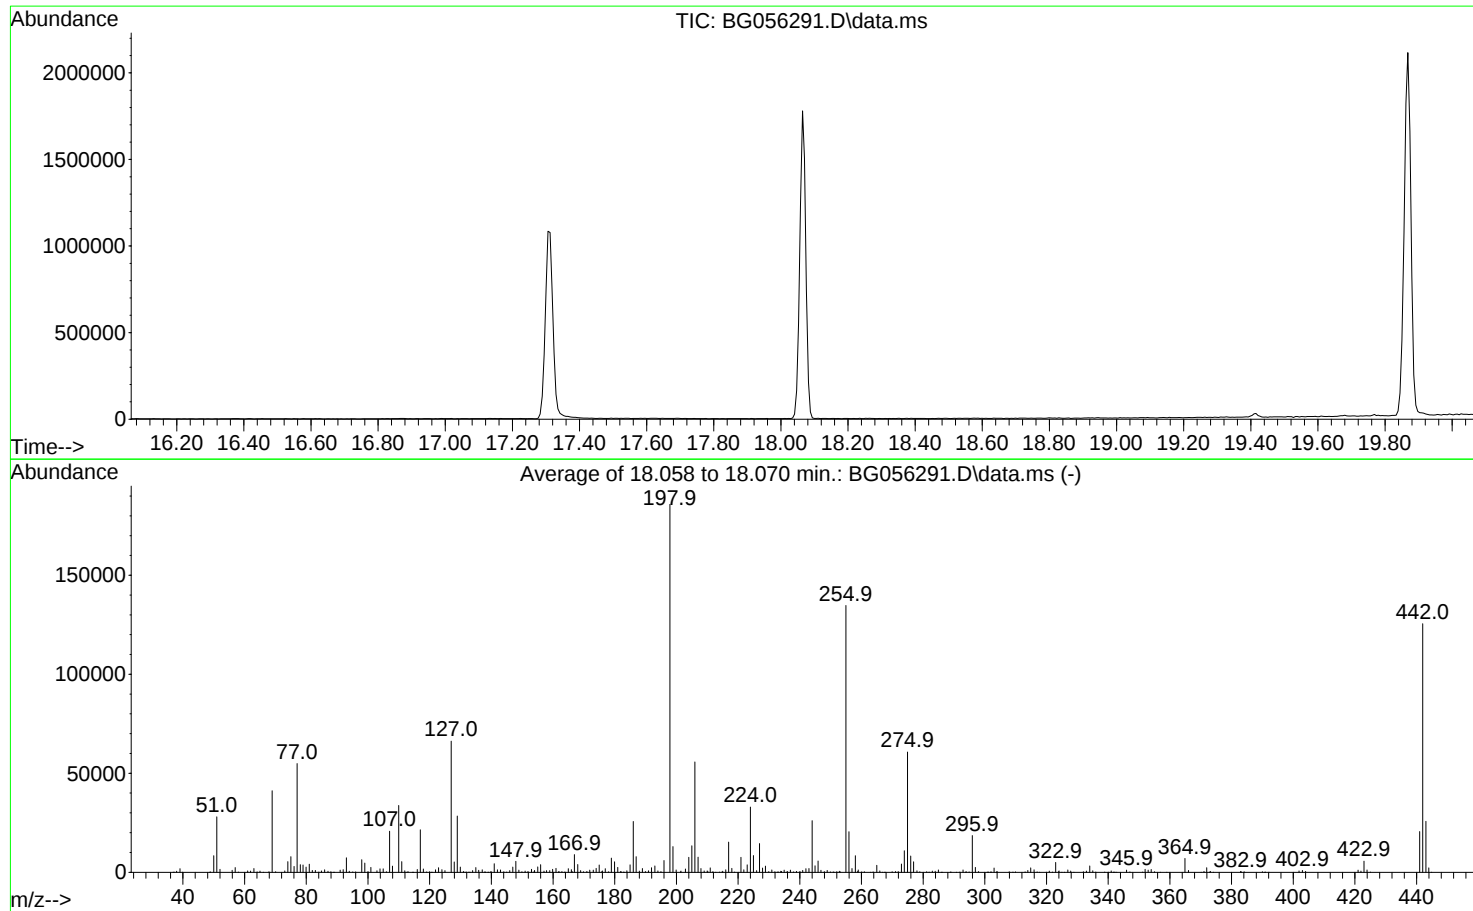




AutoFind: Scans 2514, 2515, 2516; Background Corrected with Scan 2507

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	15.1	27981	PASS
68	69	0.00	2	0.6	263	PASS
69	198	0.00	100	22.2	41195	PASS
70	69	0.00	2	0.6	266	PASS
127	198	10	80	35.7	66261	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	185771	PASS
199	198	5	9	7.0	12939	PASS
275	198	10	60	32.7	60757	PASS
365	198	1	100	3.8	7017	PASS
441	198	0.01	100	11.1	20549	PASS
442	442	50	100	100.0	125573	PASS
443	442	15	24	20.5	25725	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011623\
Data File : BG056291.D
Acq On : 16 Jan 2023 10:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 17 07:48:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 12 03:38:40 2023
Response via : Initial Calibration

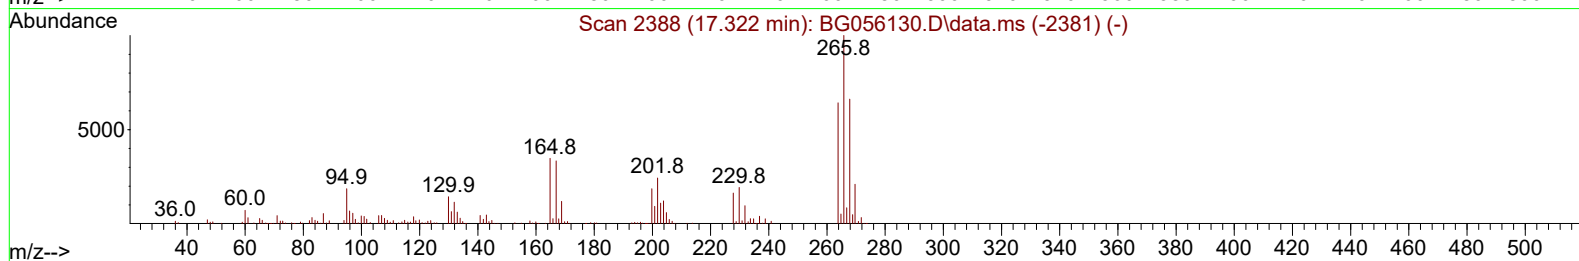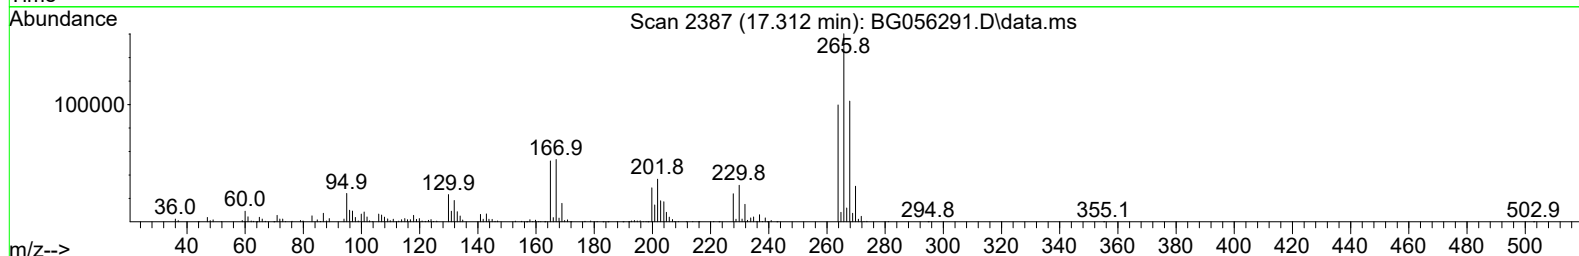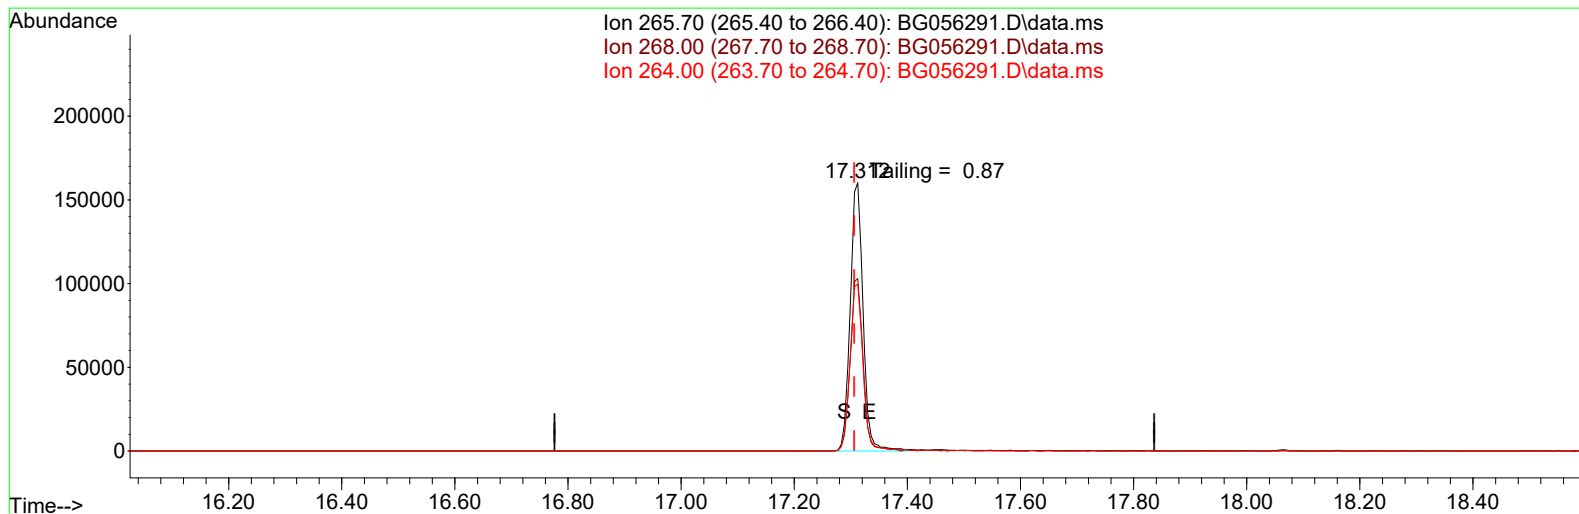

TIC: BG056291.D\data.ms

(70) Pentachlorophenol (C)

17.312min (+ 0.006) 306489.16 ng




response 254536

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.20	64.22
264.00	64.30	62.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011623\
Data File : BG056291.D
Acq On : 16 Jan 2023 10:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 17 07:48:41 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 12 03:38:40 2023
Response via : Initial Calibration

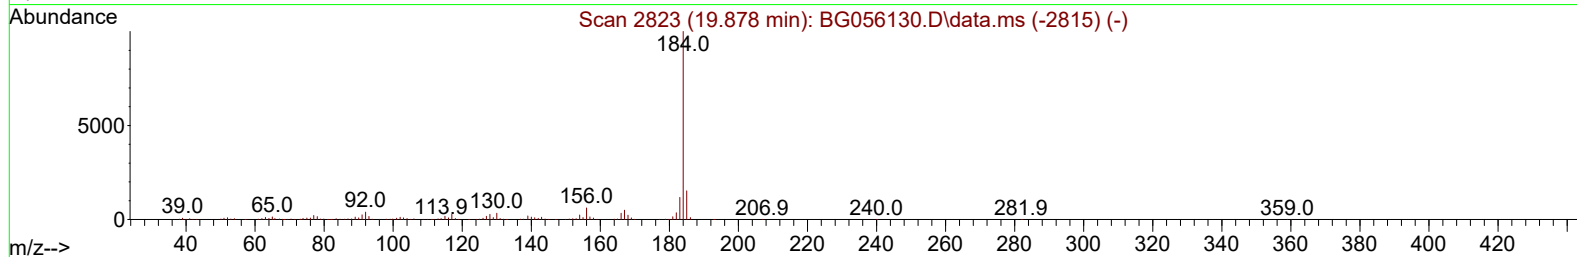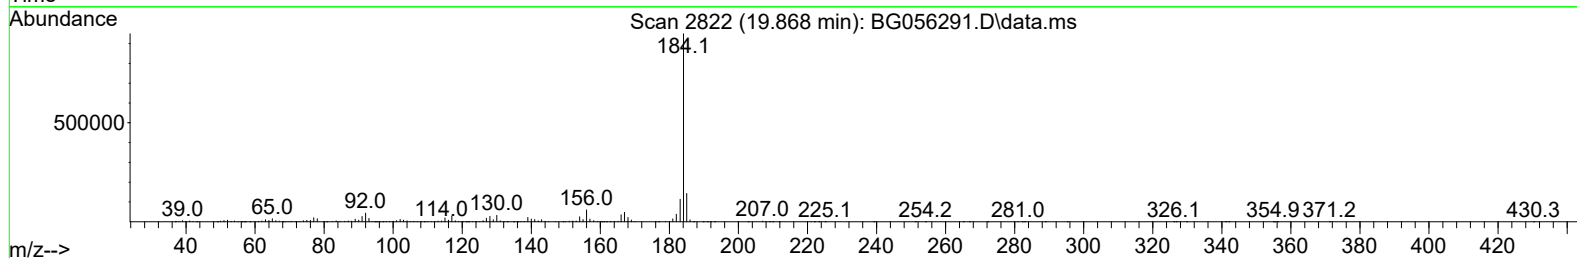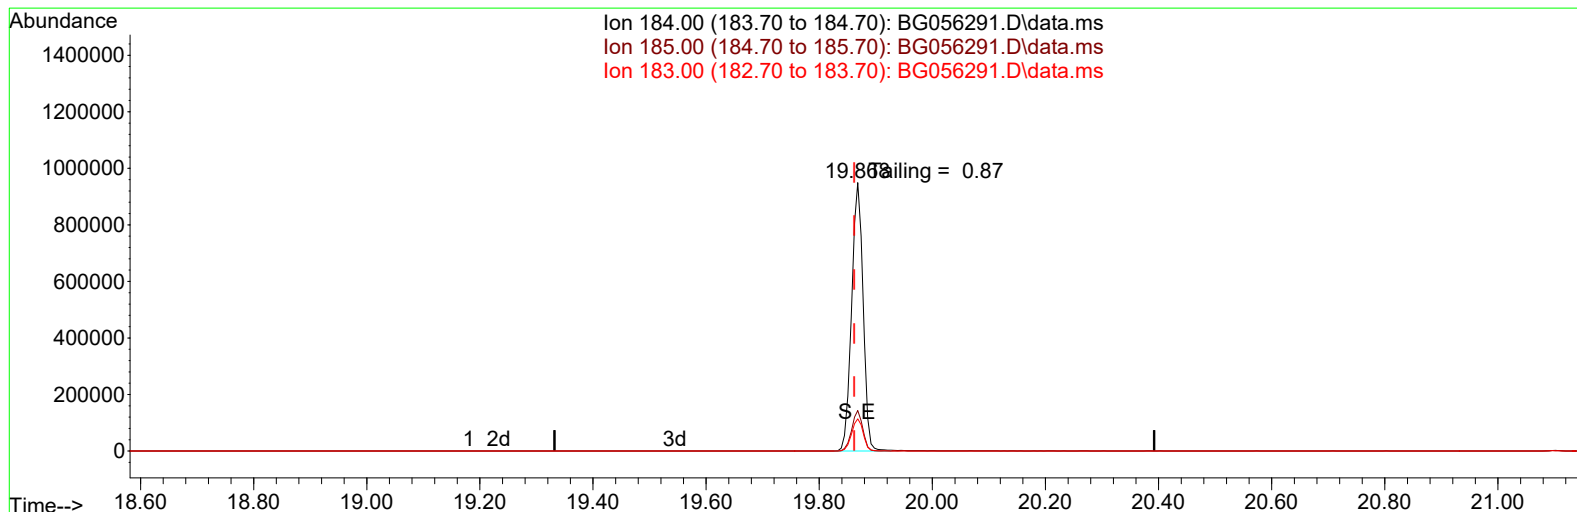

TIC: BG056291.D\data.ms

(77) Benzidine

19.868min (+ 0.006) 126234.37 ng m

response 1344834

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	15.09
183.00	11.70	11.98
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/16/2023	BNA_G	<u>BG056291.D</u>
Compound Name	Response	Retention Time
DDT	624037	21.102
DDD	30321	20.644
DDE	1338	20.144
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
31659	655696	4.83

Instrument :
BNA_G
ClientSampleId :
DFTPP