
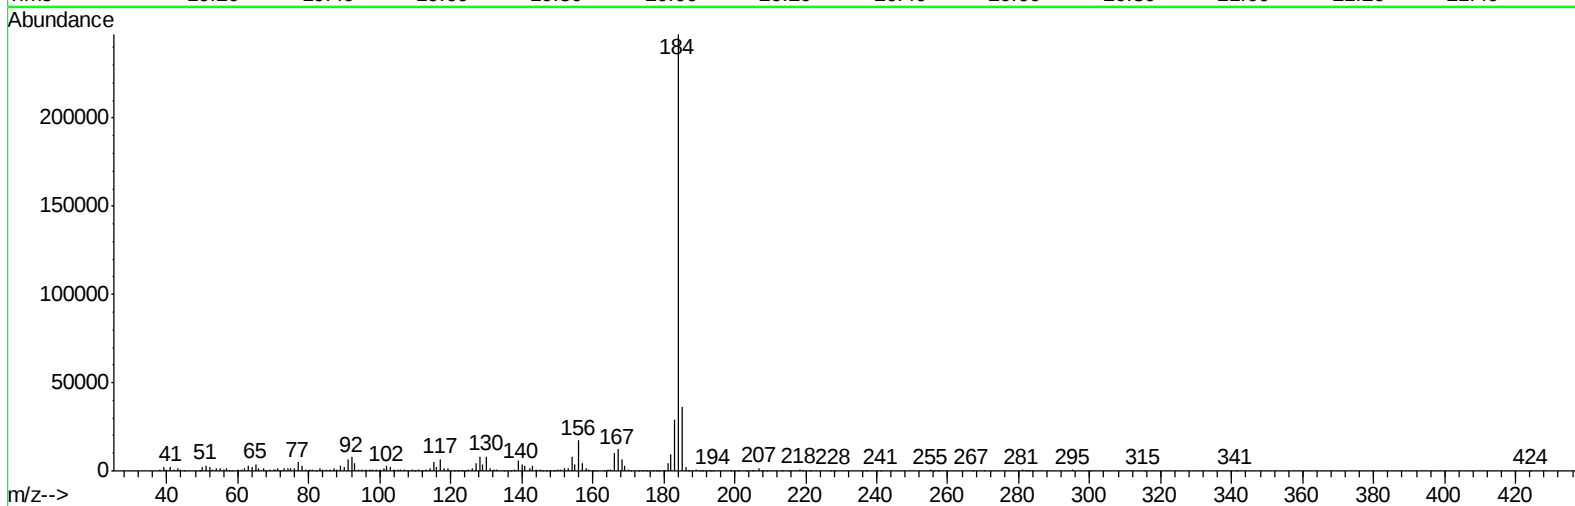


Data Path : Z:\HPCHEM1\BNA G\DATA\BG011718\
Data File : BG032105.D
Acq On : 17 Jan 2018 17:58
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 18 08:23:22 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG011218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 15 10:05:15 2018
Response via : Initial Calibration

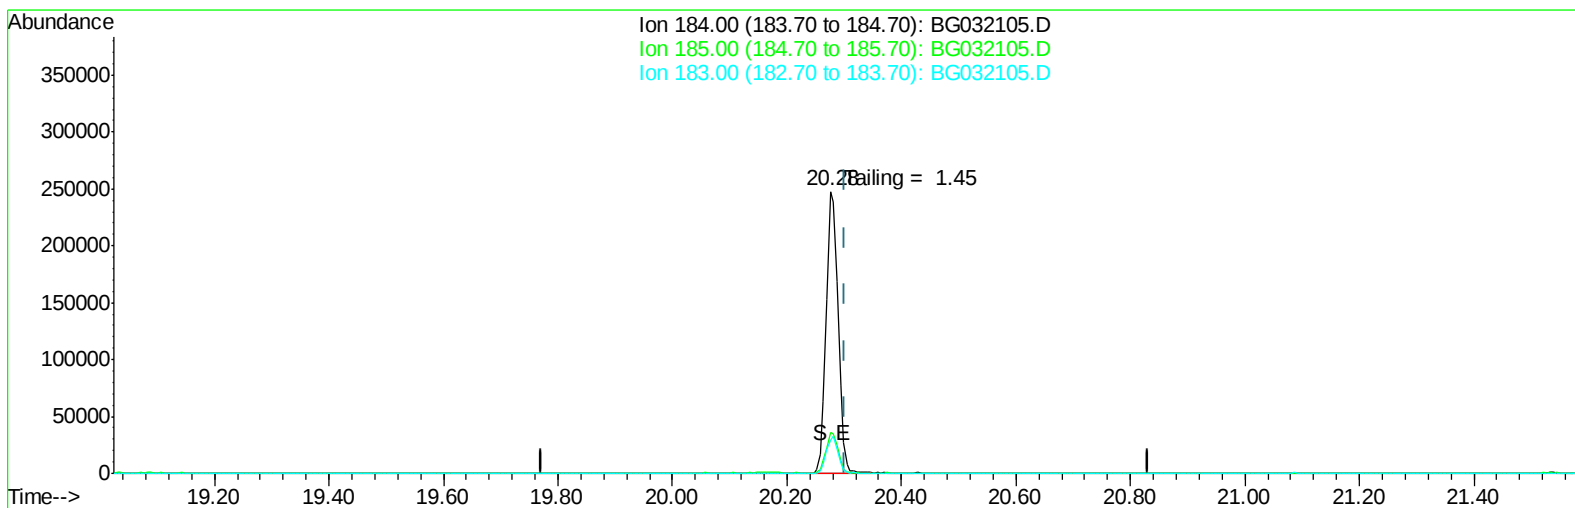

TIC: BG032105.D

(76) Benzidine



20.276min (-0.027) 1923.30ng

response 357871

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.74
183.00	13.30	11.72
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG011718\
Data File : BG032105.D
Acq On : 17 Jan 2018 17:58
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 18 08:23:22 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG011218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 15 10:05:15 2018
Response via : Initial Calibration

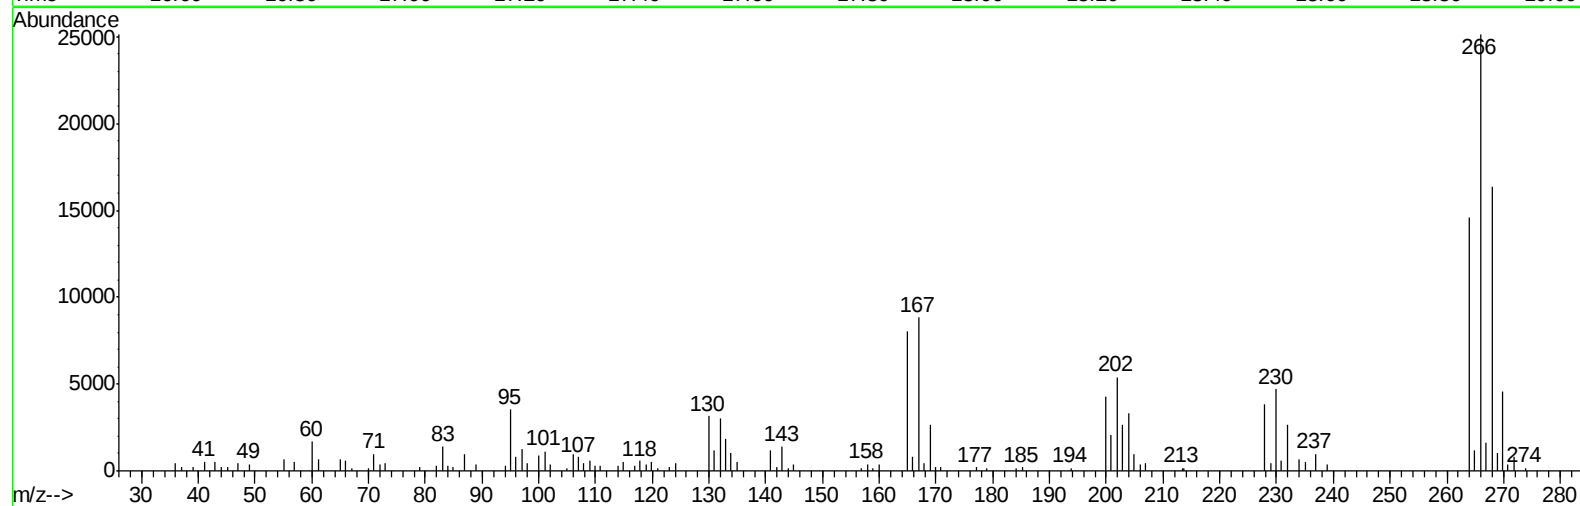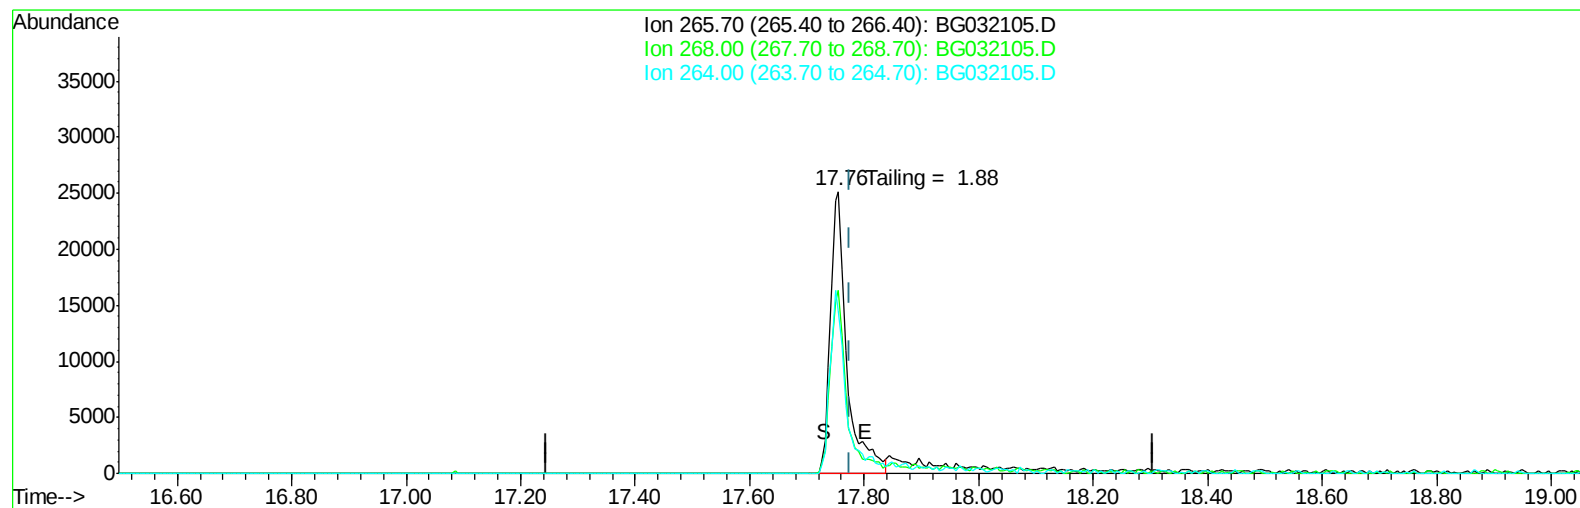

TIC: BG032105.D

(69) Pentachlorophenol (C)

17.755min (-0.021) 89530.25ng

response 49545

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	65.16
264.00	62.00	57.95
0.00	0.00	0.00