
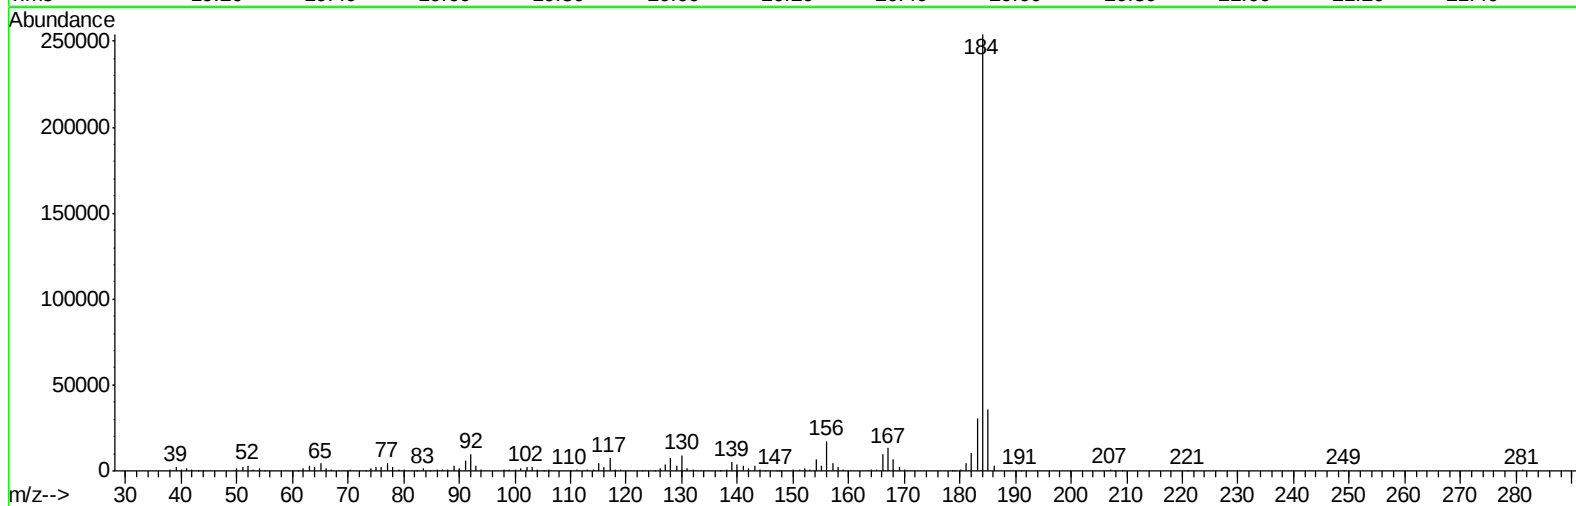


Data Path : Z:\HPCHEM1\BNA G\DATA\BG011718\
Data File : BG032124.D
Acq On : 18 Jan 2018 5:50
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 18 08:24:13 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG011218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 15 10:05:15 2018
Response via : Initial Calibration

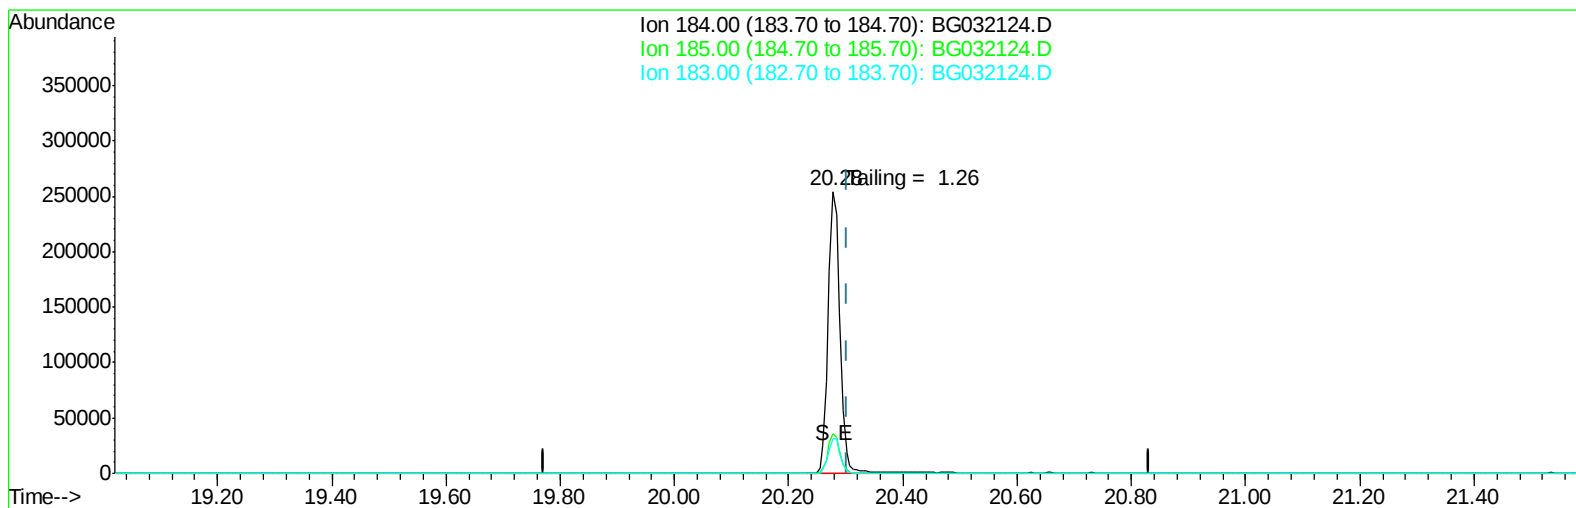

TIC: BG032124.D

(76) Benzidine



20.277min (-0.025) 78502.30ng

response 363163

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	13.98
183.00	13.30	12.18
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG011718\
Data File : BG032124.D
Acq On : 18 Jan 2018 5:50
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 18 08:24:13 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG011218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 15 10:05:15 2018
Response via : Initial Calibration

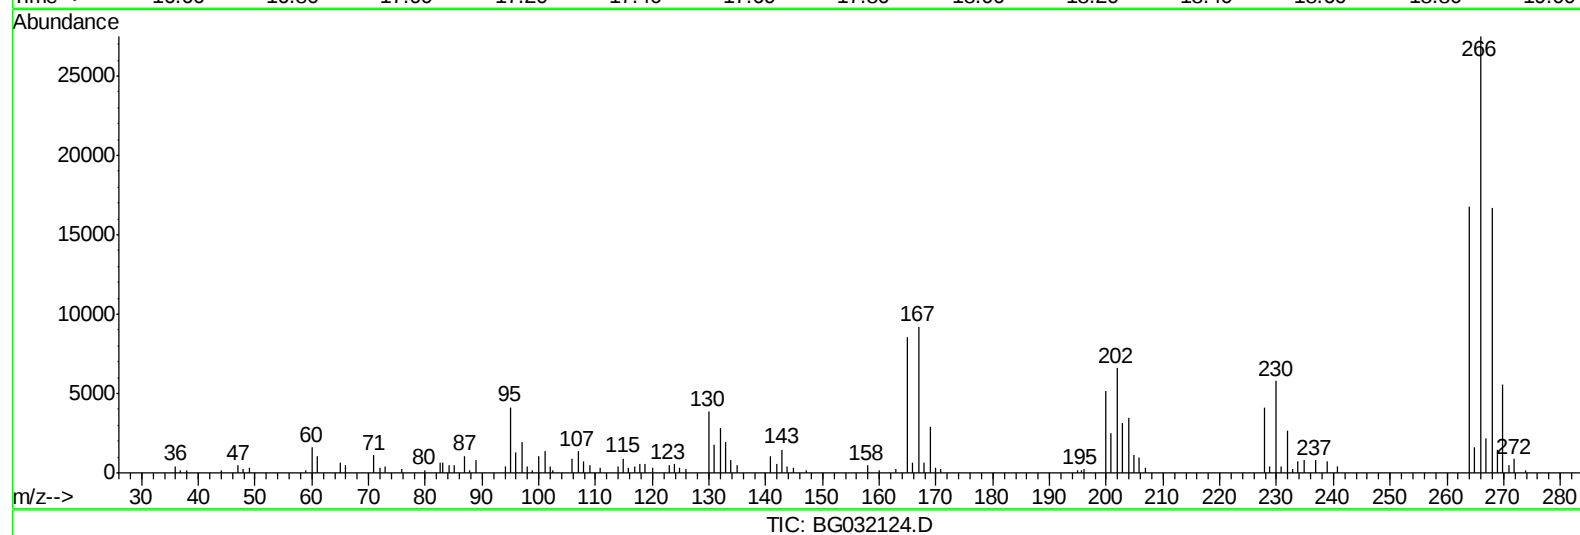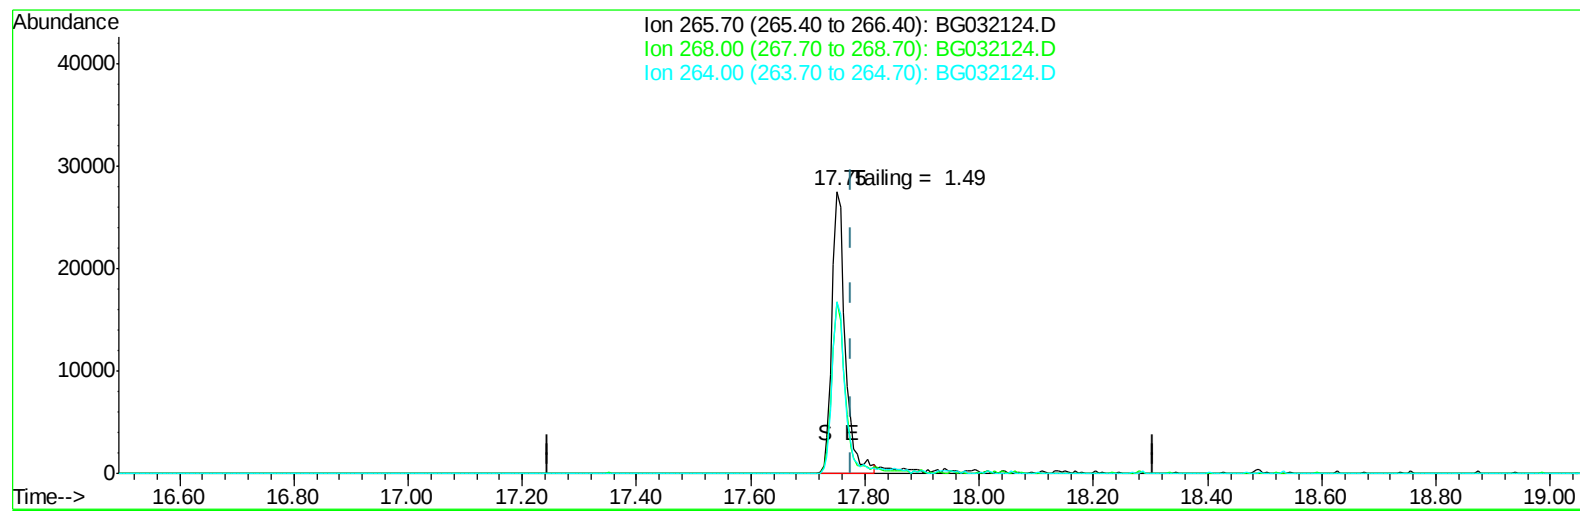

(69) Pentachlorophenol (C)

17.751min (-0.025) 13359.49ng

response 43417

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	60.73
264.00	62.00	60.97
0.00	0.00	0.00