


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA_G\Data\BG011718\
 Data File : BG032105.D
 Acq On : 17 Jan 2018 17:58
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG011218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 18 10:13:16 2018

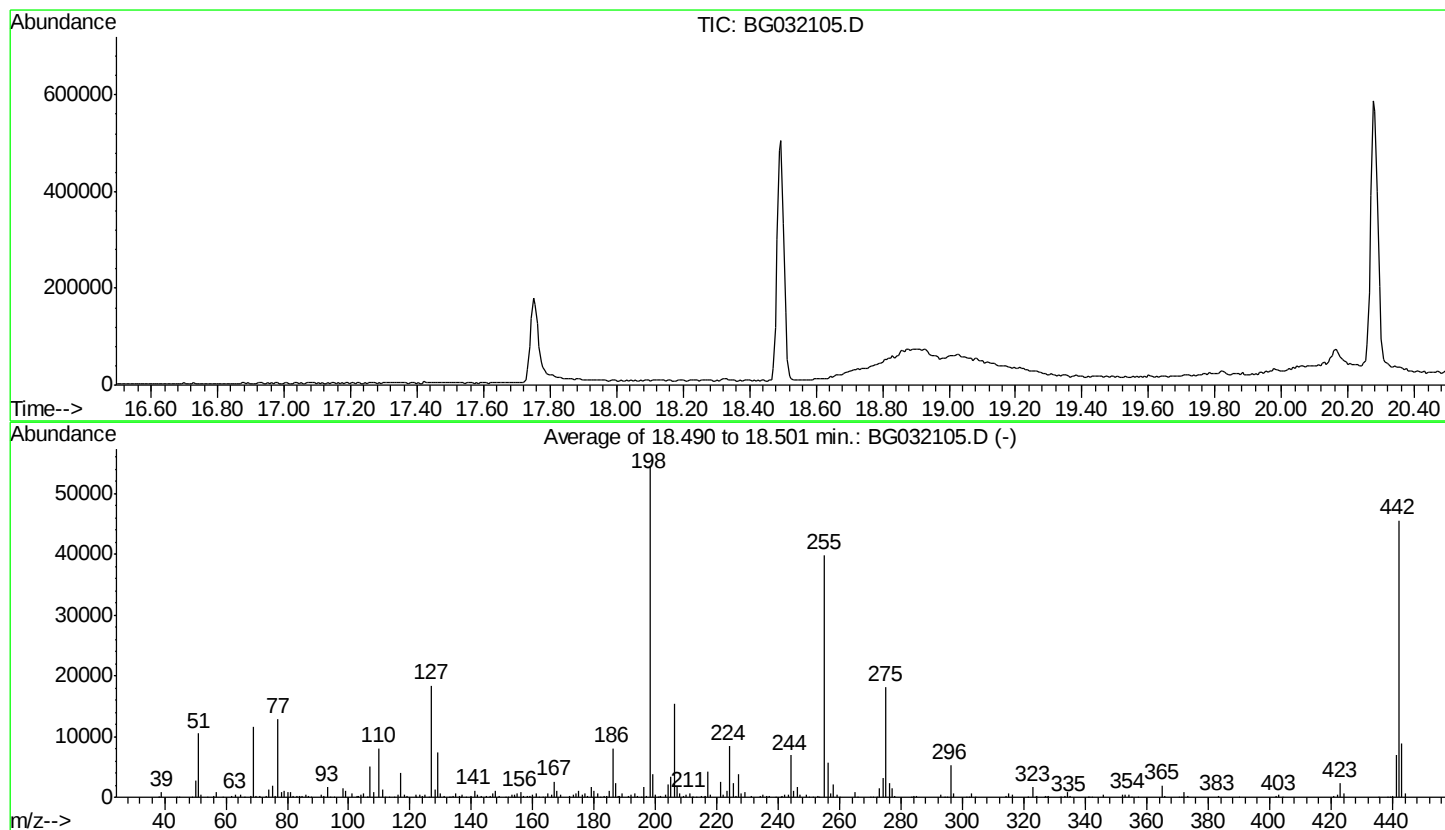

AutoFind: Scans 2587, 2588, 2589; Background Corrected with Scan 2580

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	19.1	10455	PASS
68	69	0.00	2	1.4	165	PASS
69	198	0.00	100	21.2	11577	PASS
70	69	0.00	2	1.8	209	PASS
127	198	10	80	33.7	18383	PASS
197	198	0.00	2	0.4	238	PASS
198	198	100	100	100.0	54624	PASS
199	198	5	9	7.1	3881	PASS
275	198	10	60	33.4	18235	PASS
365	198	1	100	3.7	1997	PASS
441	442	0.01	24	15.5	7067	PASS
442	198	50	100	83.4	45565	PASS
443	442	15	24	19.5	8895	PASS