
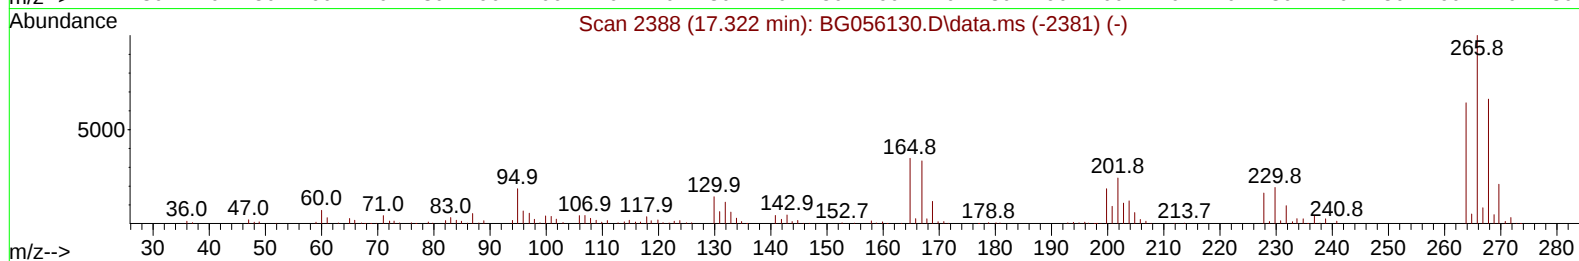
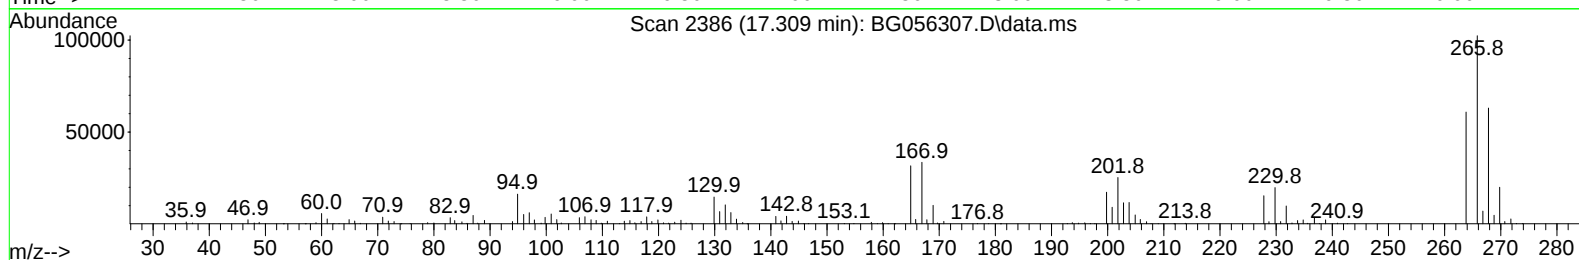


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011723\
Data File : BG056307.D
Acq On : 17 Jan 2023 9:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 18 04:02:44 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 12 03:38:40 2023
Response via : Initial Calibration

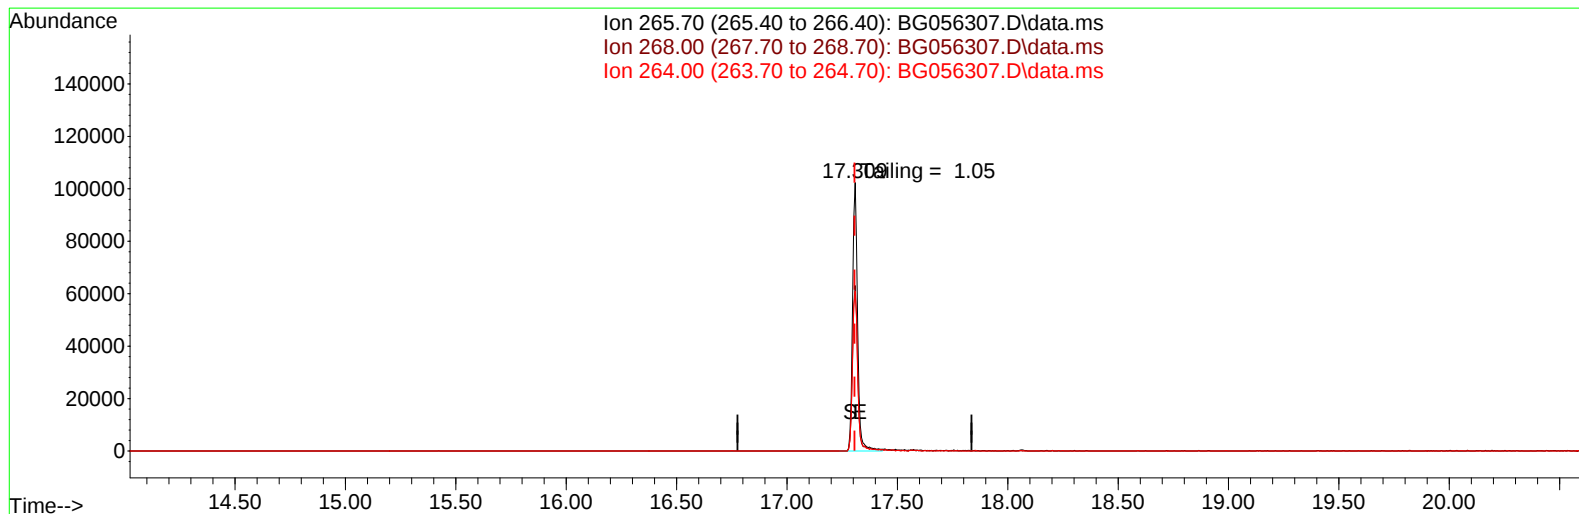

TIC: BG056307.D\data.ms

(70) Pentachlorophenol (C)




17.309min (+ 0.002) 23039.55 ng

response 159591

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.20	61.57
264.00	64.30	59.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011723\
Data File : BG056307.D
Acq On : 17 Jan 2023 9:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 18 04:02:44 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 12 03:38:40 2023
Response via : Initial Calibration

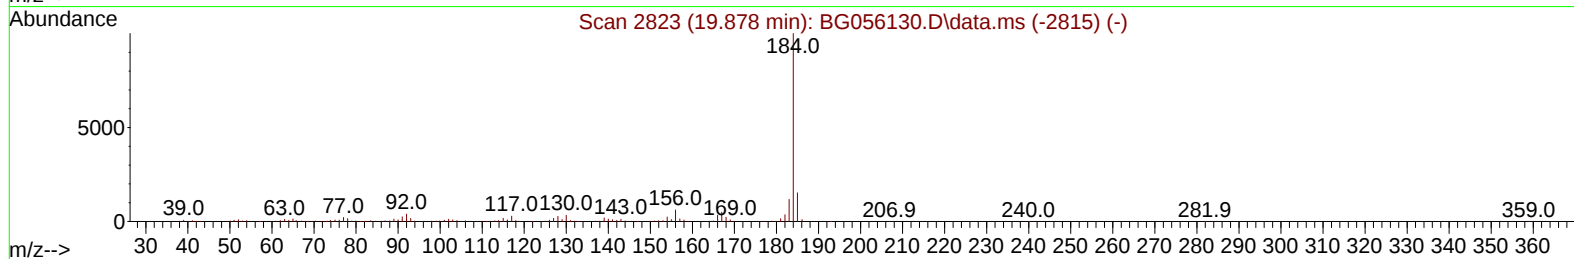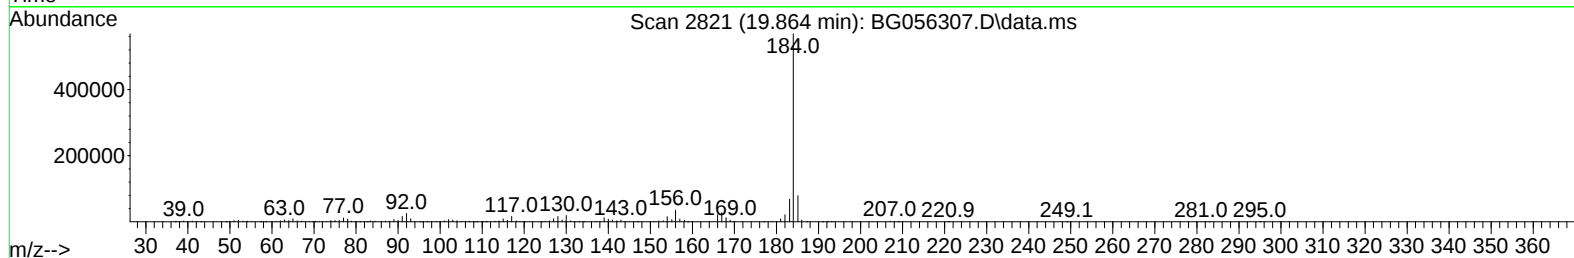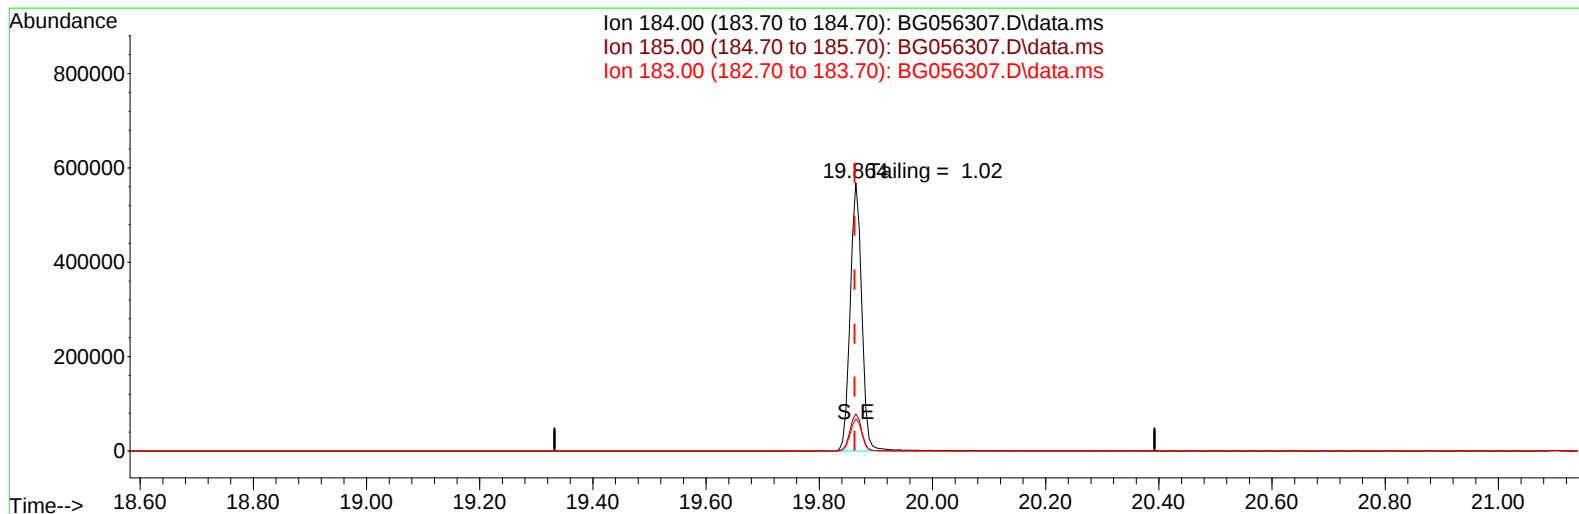

TIC: BG056307.D\data.ms

(77) Benzidine

19.864min (+ 0.002) 0.00 ng

response 807781

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	13.87
183.00	11.70	12.04
0.00	0.00	0.00