

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011723\
 Data File : BG056309.D
 Acq On : 17 Jan 2023 10:49
 Operator : CG/JU
 Sample : PB150221BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB150221BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG056309.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.351	345	351	359	rBV	148735	233100	5.44%	1.465%
2	5.833	426	433	443	rBV	672236	1061652	24.80%	6.672%
3	7.449	700	708	719	rBV	656897	1130484	26.41%	7.105%
4	8.312	846	855	863	rBB	158110	263034	6.14%	1.653%
5	9.488	1045	1055	1063	rBV	389194	685461	16.01%	4.308%
6	11.144	1330	1337	1347	rVB	212257	381916	8.92%	2.400%
7	13.553	1740	1747	1758	rBV	1604576	2466355	57.61%	15.500%
8	14.928	1973	1981	1989	rBV	430529	683849	15.97%	4.298%
9	16.403	2225	2232	2244	rBV	1120482	1729083	40.39%	10.867%
10	17.660	2440	2446	2454	rBV	604067	906693	21.18%	5.698%
11	20.240	2879	2885	2891	rBV	3307741	4280998	100.00%	26.904%
12	21.955	3170	3177	3187	rVB	592001	1042387	24.35%	6.551%
13	25.398	3752	3763	3775	rBV2	339458	1046990	24.46%	6.580%




Sum of corrected areas: 15912002

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011723\
Data File : BG056309.D
Acq On : 17 Jan 2023 10:49
Operator : CG/JU
Sample : PB150221BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB150221BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

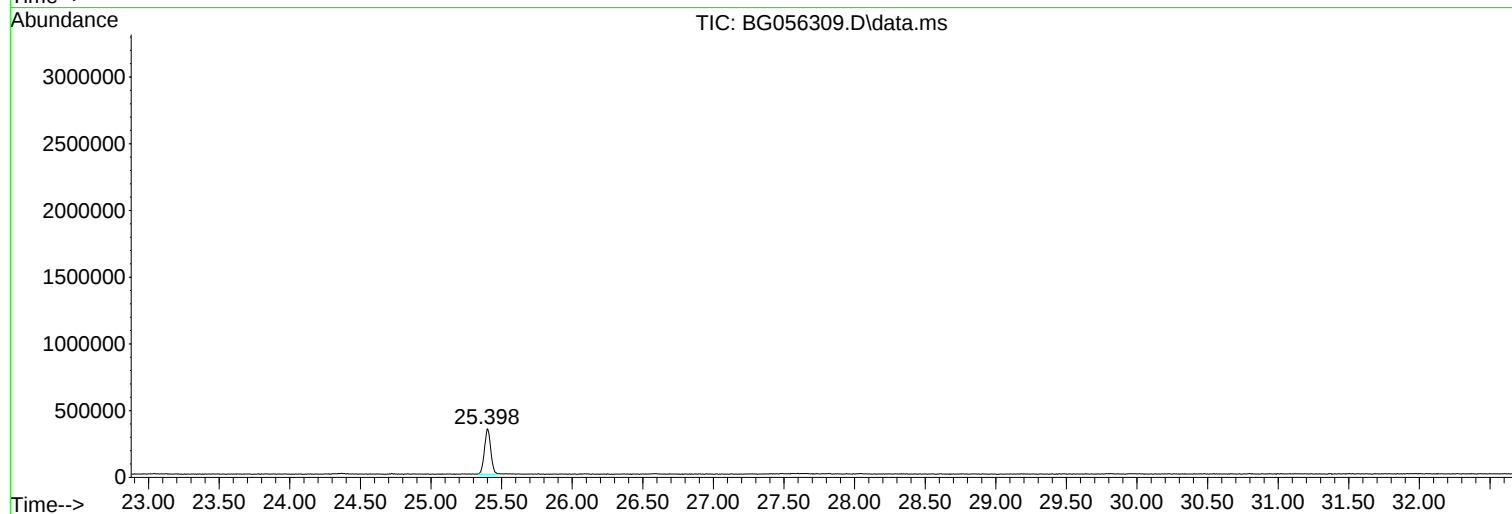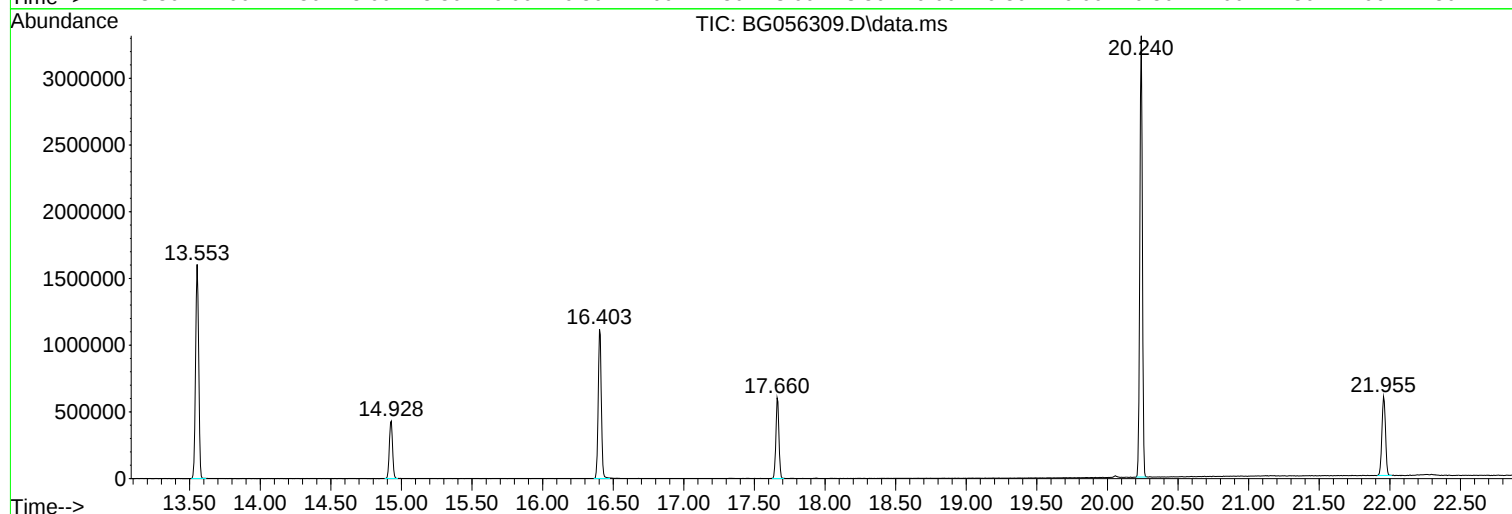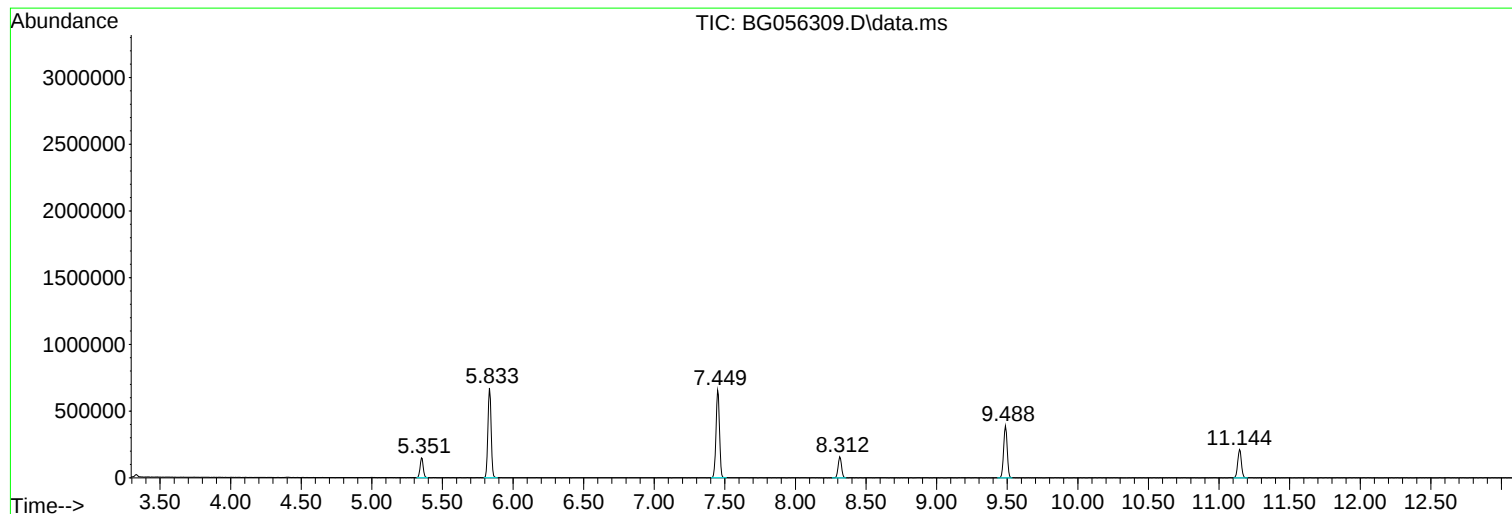

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011723\
Data File : BG056309.D
Acq On : 17 Jan 2023 10:49
Operator : CG/JU
Sample : PB150221BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB150221BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.351	17.72 ng	233100	1,4-Dichlorobenzene-d4	8.318

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	50		
2	Guanidine	59	CH5N3	000113-00-8	37		
3	Propane, 1-ethoxy-2-methyl-	102	C6H14O	000627-02-1	35		
4	Butyl aldoxime, 3-methyl-, syn-	101	C5H11NO	005780-40-5	35		
5	4-Methoxy-1-pentene	100	C6H12O	098386-09-5	35		

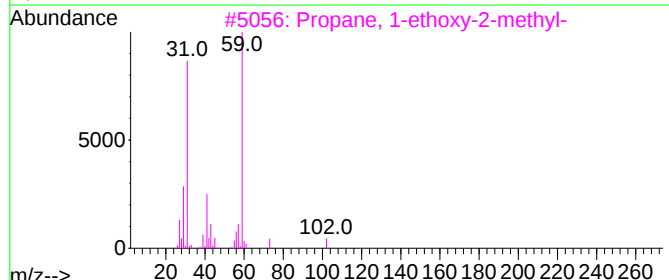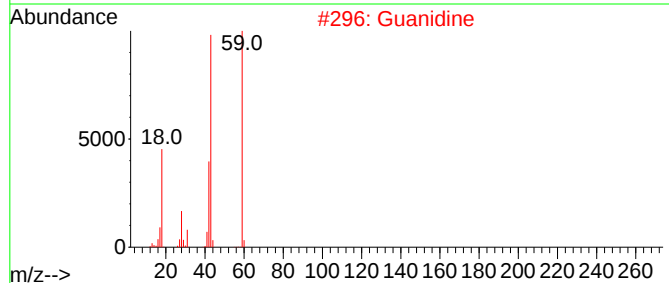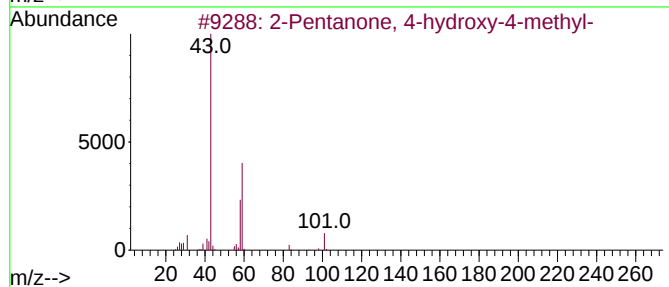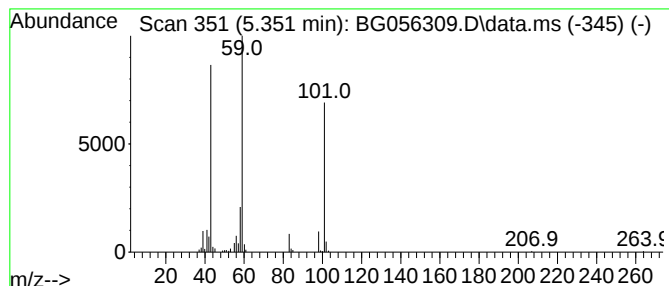

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011723\
Data File : BG056309.D
Acq On : 17 Jan 2023 10:49
Operator : CG/JU
Sample : PB150221BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB150221BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.351	17.7	ng	233100	1	8.318	263034	20.0