

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011723\
 Data File : BG056313.D
 Acq On : 17 Jan 2023 13:40
 Operator : CG/JU
 Sample : 01140-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 TP-D

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG056313.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.347	5	10	25	rVB	403532	670640	14.86%	4.533%
2	4.734	240	246	254	rBV	229351	324192	7.18%	2.191%
3	5.357	348	352	358	rVB	69981	107967	2.39%	0.730%
4	5.833	426	433	443	rVB	632442	996771	22.09%	6.737%
5	7.448	702	708	720	rVB	538977	953308	21.13%	6.443%
6	8.312	846	855	866	rVB	107847	186337	4.13%	1.259%
7	9.487	1046	1055	1064	rBV	379159	686298	15.21%	4.639%
8	11.144	1330	1337	1348	rVB	137904	246664	5.47%	1.667%
9	13.553	1739	1747	1754	rBV	1457112	2202632	48.81%	14.887%
10	14.928	1974	1981	1988	rBV	241471	381002	8.44%	2.575%
11	16.403	2226	2232	2249	rBV	1063819	1659133	36.77%	11.214%
12	17.660	2440	2446	2459	rVB	385685	592108	13.12%	4.002%
13	18.506	2582	2590	2599	rBV3	36483	61003	1.35%	0.412%
14	19.763	2798	2804	2813	rBV3	31027	51635	1.14%	0.349%
15	20.239	2879	2885	2891	rBV	3564867	4512268	100.00%	30.498%
16	21.955	3171	3177	3190	rVB2	432028	752644	16.68%	5.087%
17	25.404	3754	3764	3775	rBV3	120003	410816	9.10%	2.777%




Sum of corrected areas: 14795418

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011723\
Data File : BG056313.D
Acq On : 17 Jan 2023 13:40
Operator : CG/JU
Sample : 01140-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-D

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

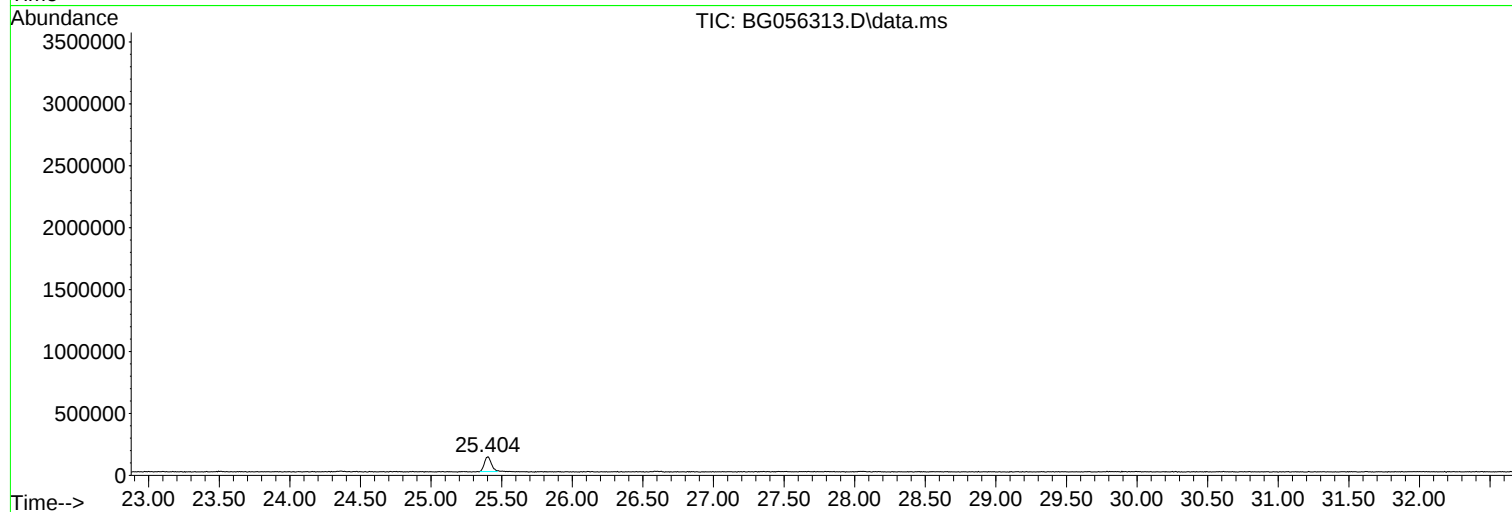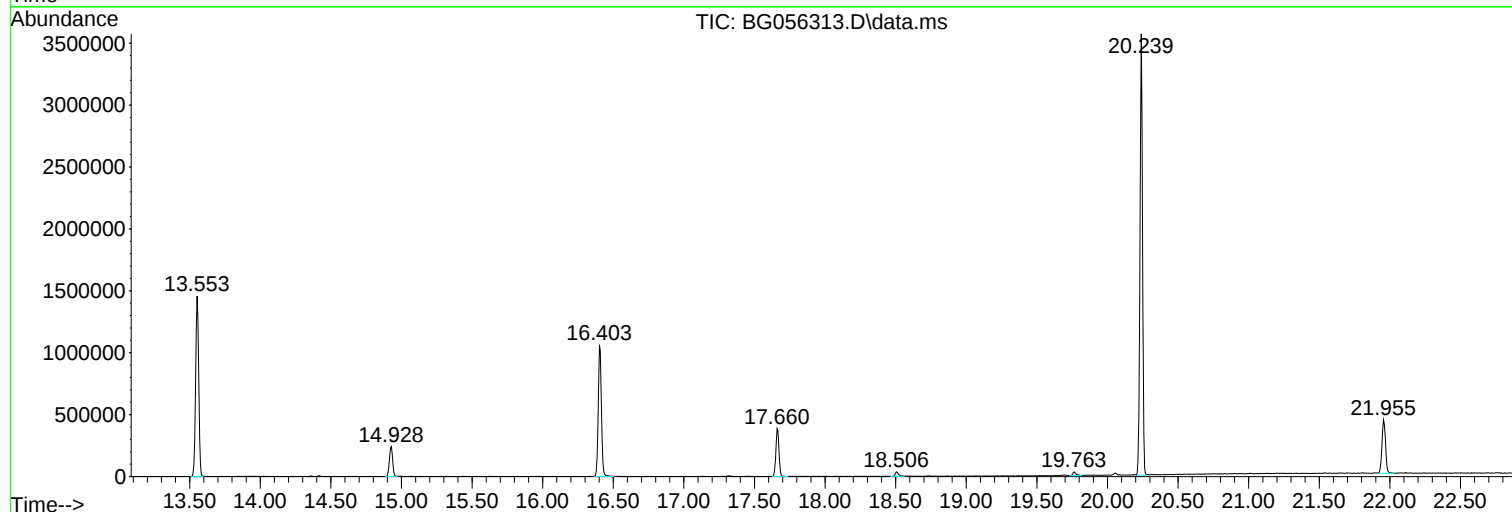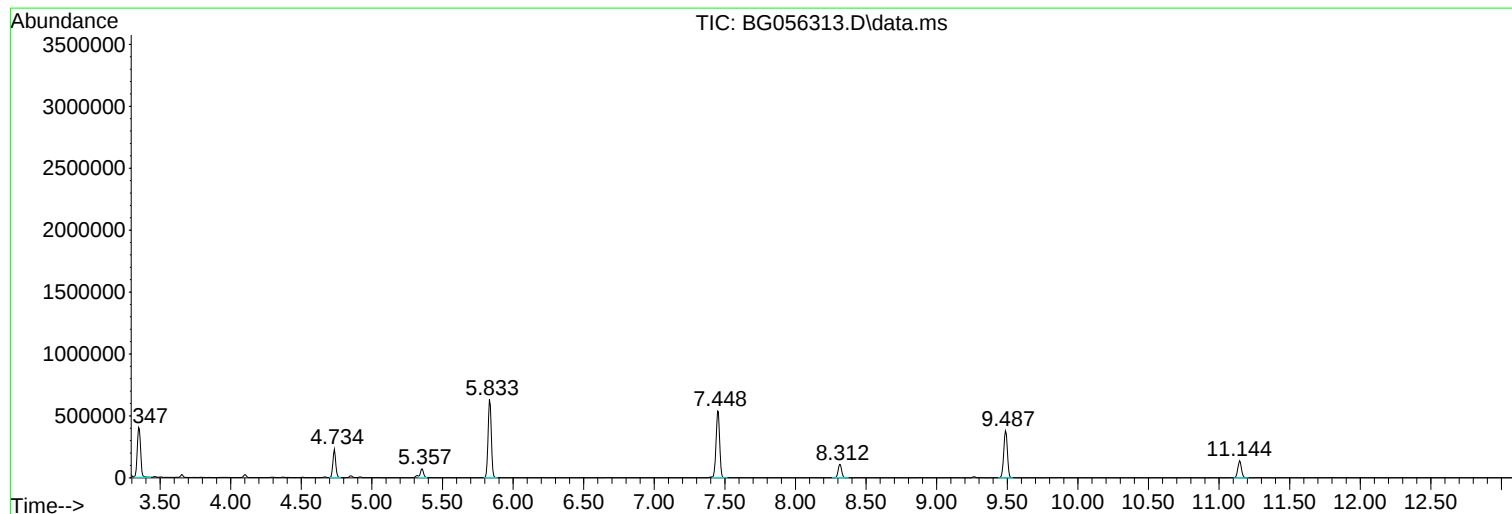

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011723\
Data File : BG056313.D
Acq On : 17 Jan 2023 13:40
Operator : CG/JU
Sample : 01140-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-D

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011723\
Data File : BG056313.D
Acq On : 17 Jan 2023 13:40
Operator : CG/JU
Sample : 01140-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-D

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------