

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011723\
 Data File : BG056319.D
 Acq On : 17 Jan 2023 18:47
 Operator : CG/JU
 Sample : 01170-01 5X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 CL-2-011623

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG056319.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.336	5	8	16	rVB2	32580	53118	5.61%	1.070%
2	5.357	347	352	360	rVB	21051	34429	3.64%	0.693%
3	5.839	426	434	442	rBV	90050	150112	15.86%	3.023%
4	7.454	700	709	718	rVB	92857	165208	17.46%	3.327%
5	8.318	848	856	864	rBV	208943	350288	37.01%	7.054%
6	9.487	1047	1055	1062	rBV2	56260	103027	10.89%	2.075%
7	11.150	1331	1338	1346	rVB	275459	485499	51.30%	9.777%
8	13.553	1739	1747	1754	rBV	213133	326927	34.54%	6.583%
9	14.928	1974	1981	1989	rBV	476745	738417	78.03%	14.870%
10	16.403	2227	2232	2239	rBV	134709	209366	22.12%	4.216%
11	17.666	2441	2447	2452	rBV	575760	882976	93.30%	17.781%
12	17.707	2452	2454	2458	rVB	22823	27128	2.87%	0.546%
13	18.512	2585	2591	2595	rBV6	34577	63258	6.68%	1.274%
14	20.239	2881	2885	2889	rBV	345264	429755	45.41%	8.654%
15	21.961	3173	3178	3188	rVB2	527125	946383	100.00%	19.058%




Sum of corrected areas: 4965891

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011723\
Data File : BG056319.D
Acq On : 17 Jan 2023 18:47
Operator : CG/JU
Sample : 01170-01 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CL-2-011623

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

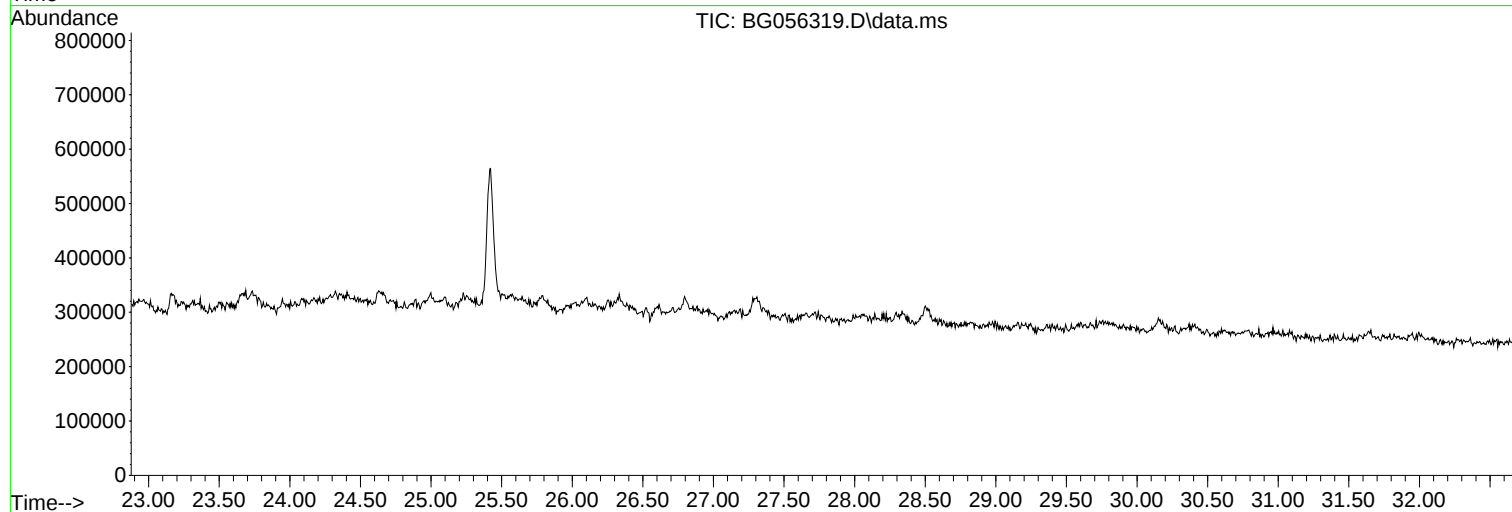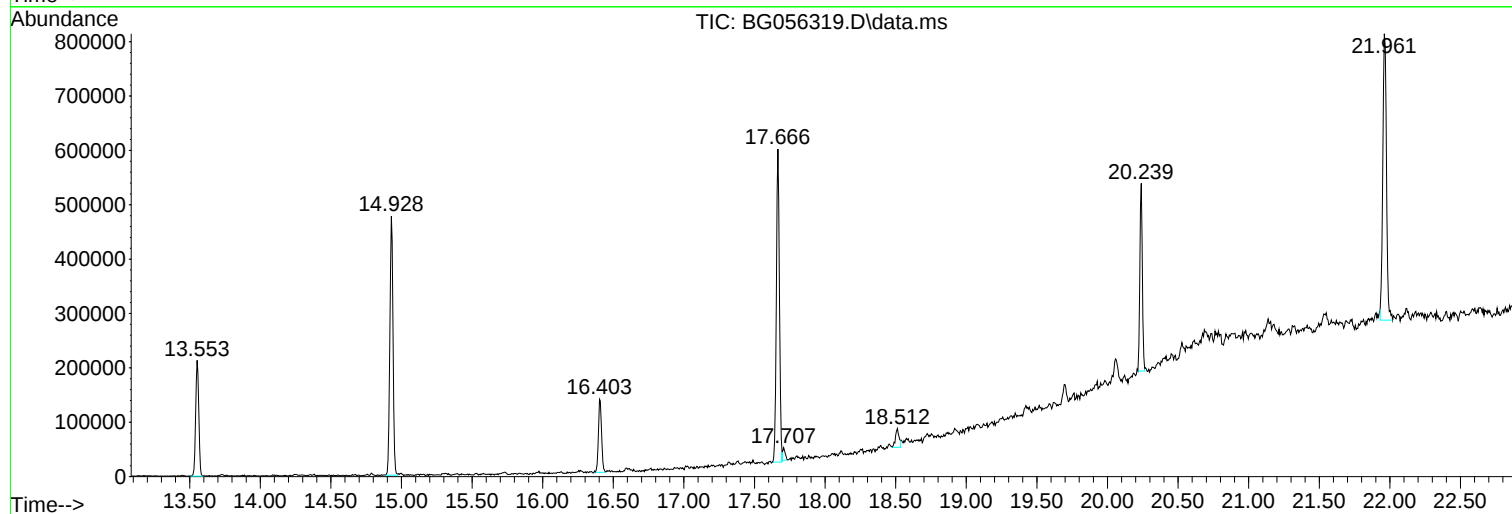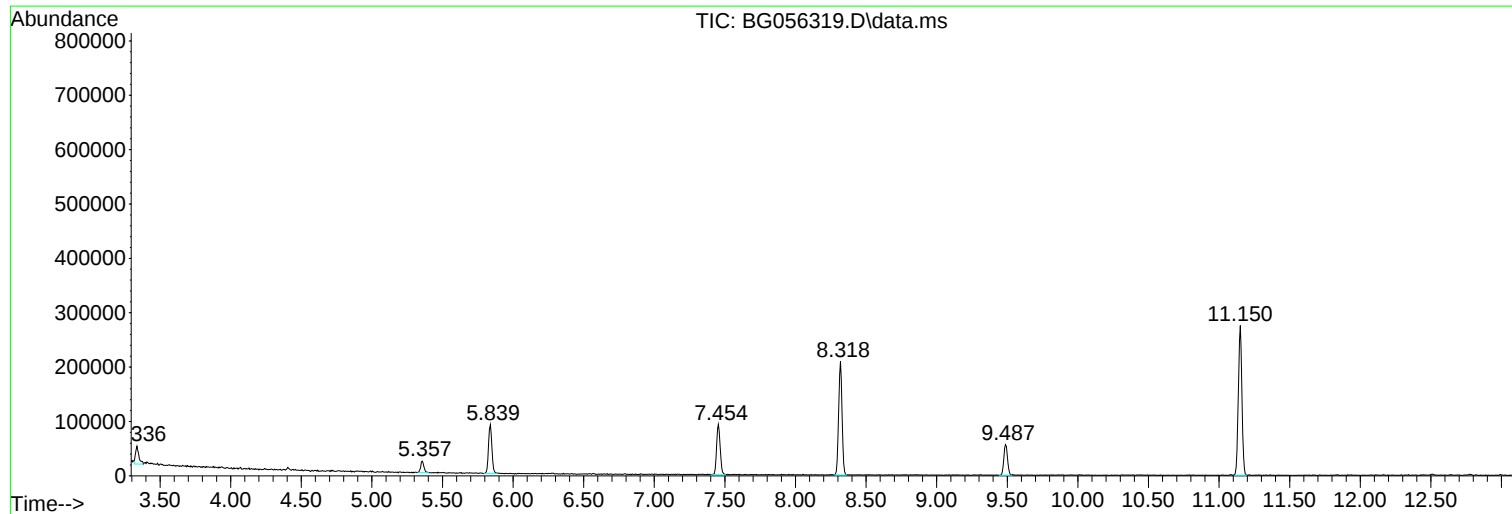

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011723\
Data File : BG056319.D
Acq On : 17 Jan 2023 18:47
Operator : CG/JU
Sample : 01170-01 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CL-2-011623










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown3.336 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.336	3.03 ng	53118	1,4-Dichlorobenzene-d4	8.318

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Hexanol, 2,4-dimethyl-	130	C8H18O	013432-25-2	25
2			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	25
3			Octanal, 7-methoxy-3,7-dimethyl-	186	C11H22O2	003613-30-7	10
4			Silane, tetramethyl-	88	C4H12Si	000075-76-3	9
5			2-(3-Methyl-3-nitrobutyl)-1,3-di...	189	C8H15NO4	057620-56-1	9

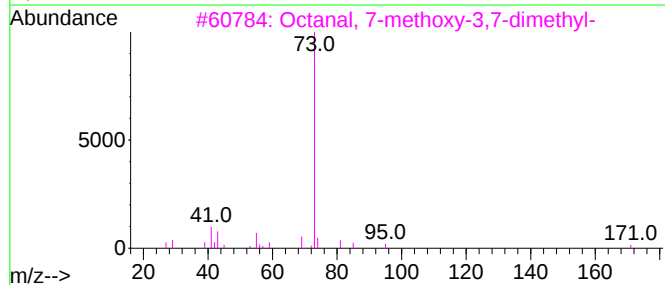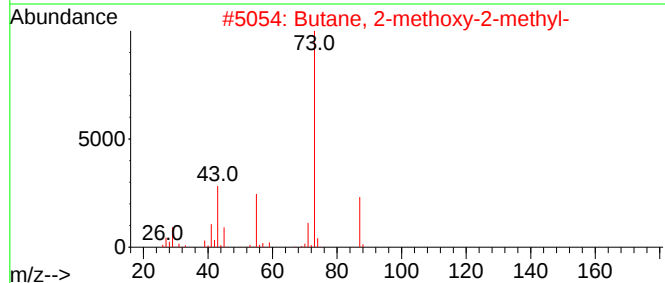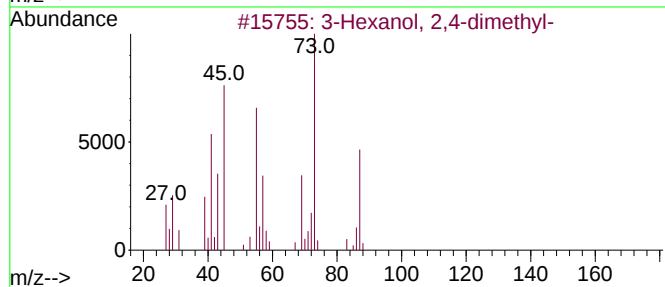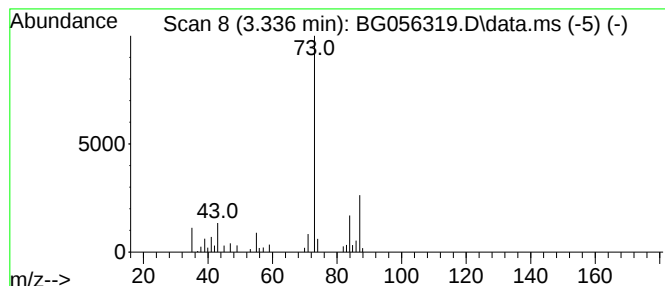

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011723\
Data File : BG056319.D
Acq On : 17 Jan 2023 18:47
Operator : CG/JU
Sample : 01170-01 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
CL-2-011623

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown3.336	3.336	3.0	ng	53118	1	8.318	350288	20.0