


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011723\
Data File : BG056307.D
Acq On : 17 Jan 2023 9:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jan 12 03:38:40 2023

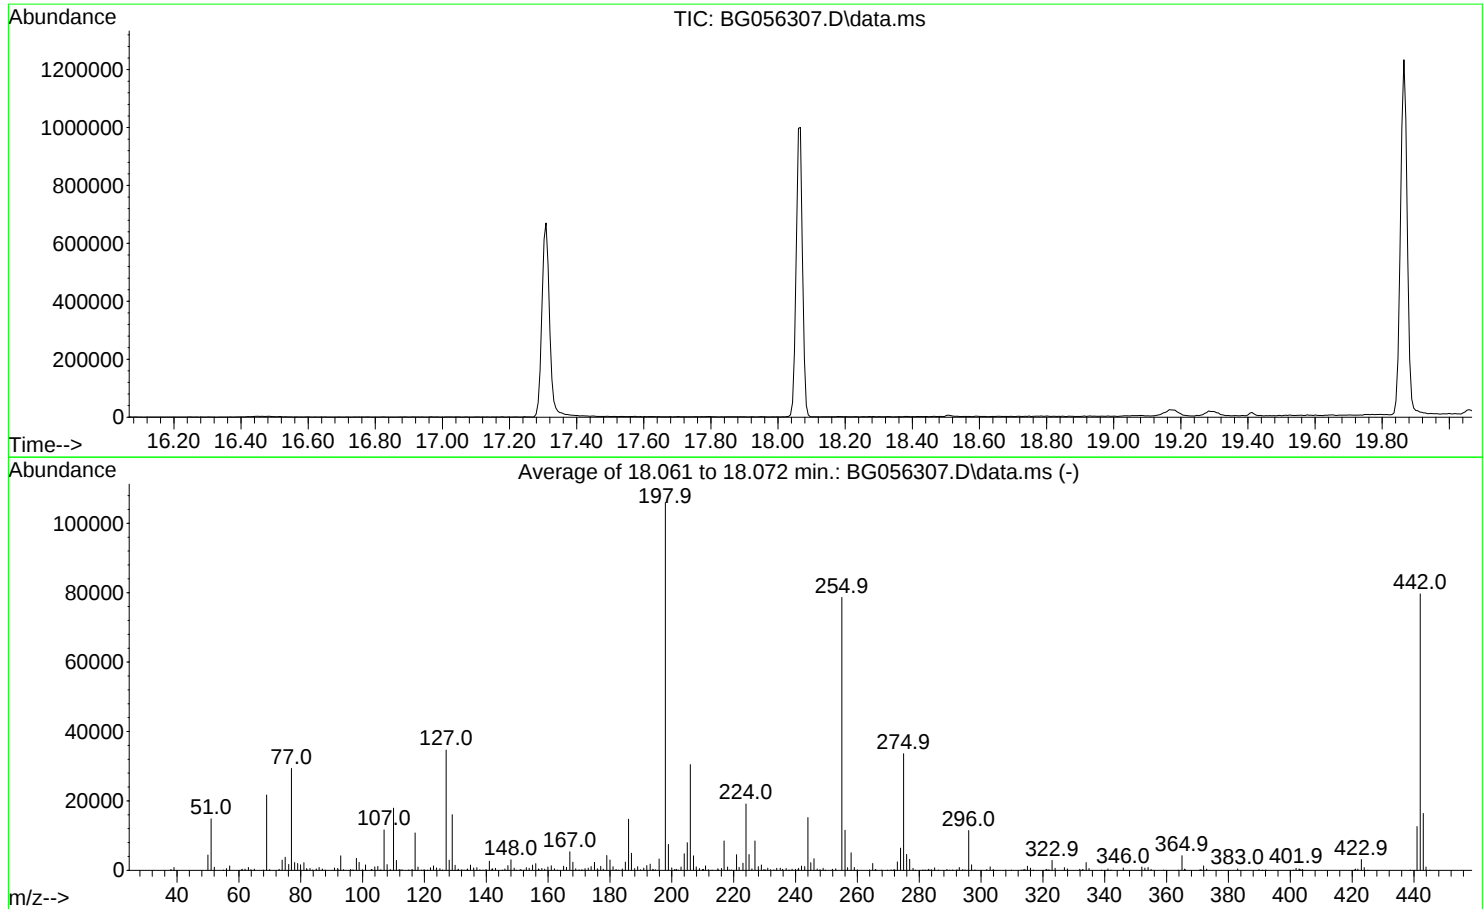




AutoFind: Scans 2514, 2515, 2516; Background Corrected with Scan 2506

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	14.0	14836	PASS
68	69	0.00	2	0.4	89	PASS
69	198	0.00	100	20.5	21719	PASS
70	69	0.00	2	1.0	218	PASS
127	198	10	80	32.7	34648	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	106019	PASS
199	198	5	9	7.0	7439	PASS
275	198	10	60	31.7	33613	PASS
365	198	1	100	4.0	4231	PASS
441	198	0.01	100	11.9	12633	PASS
442	442	50	100	100.0	79651	PASS
443	442	15	24	20.6	16383	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011723\
Data File : BG056307.D
Acq On : 17 Jan 2023 9:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 18 04:02:44 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 12 03:38:40 2023
Response via : Initial Calibration

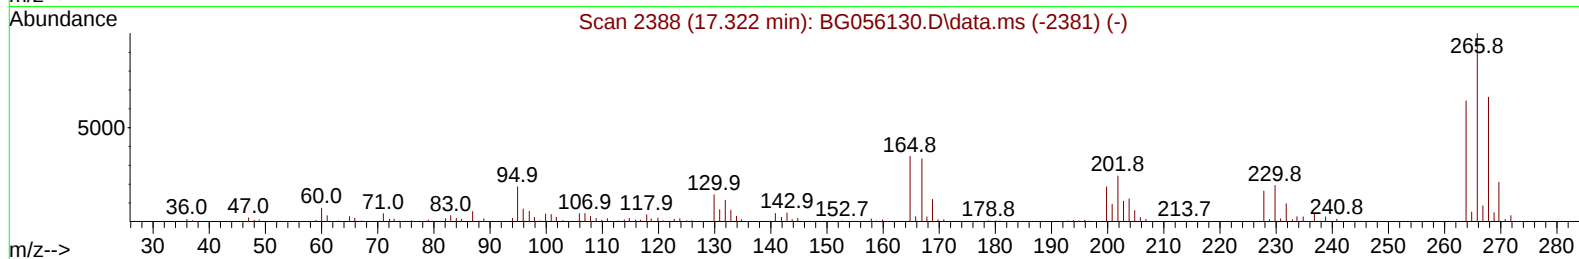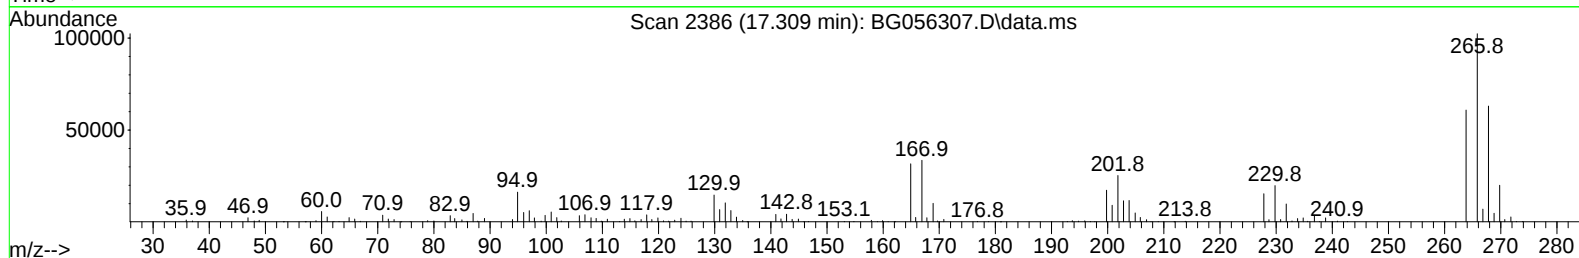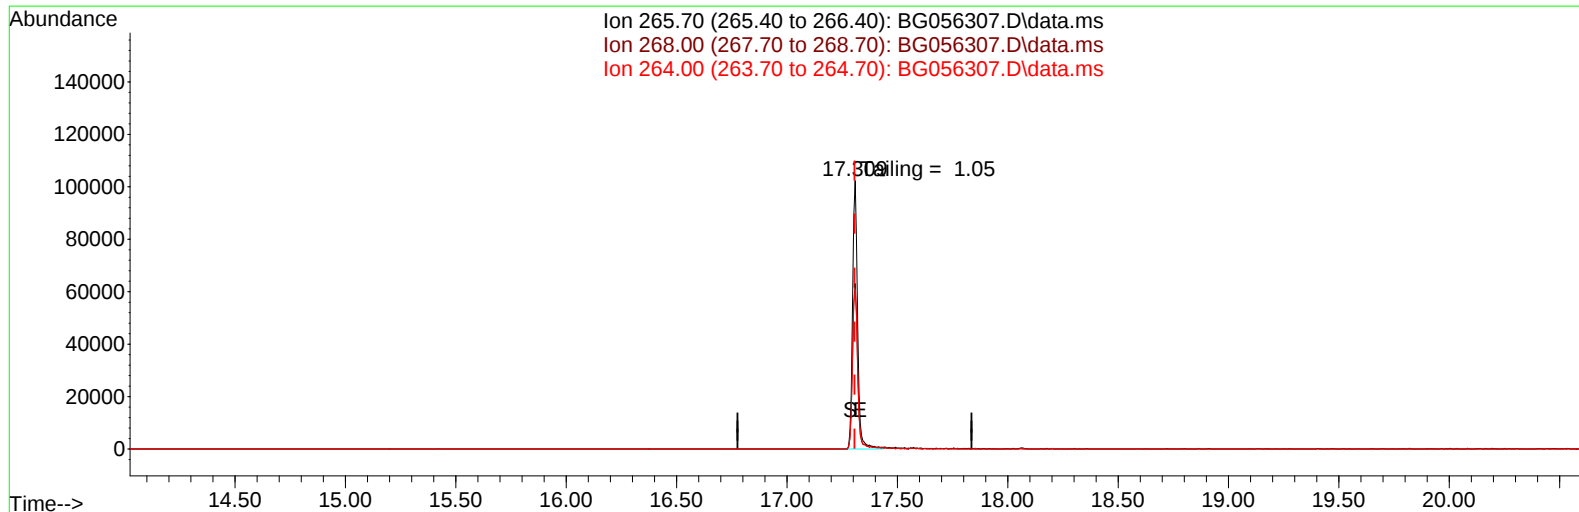

TIC: BG056307.D\data.ms

(70) Pentachlorophenol (C)

17.309min (+ 0.002) 23039.55 ng




response 159591

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.20	61.57
264.00	64.30	59.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011723\
Data File : BG056307.D
Acq On : 17 Jan 2023 9:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 18 04:02:44 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 12 03:38:40 2023
Response via : Initial Calibration

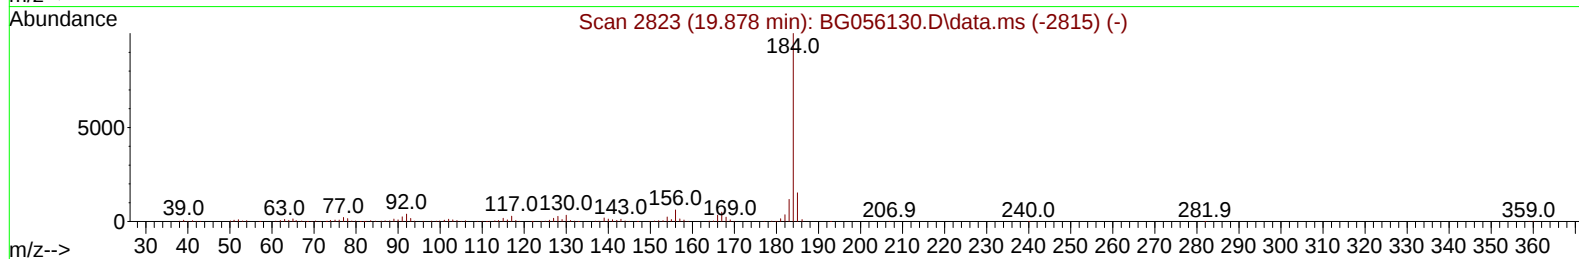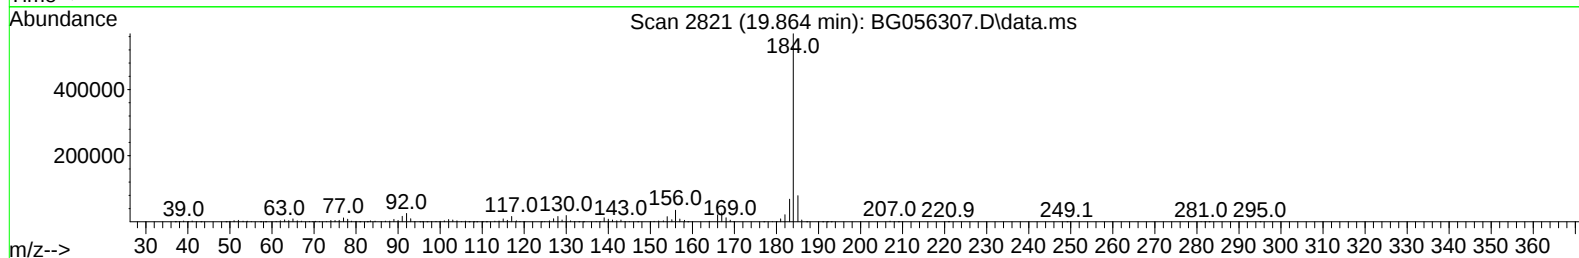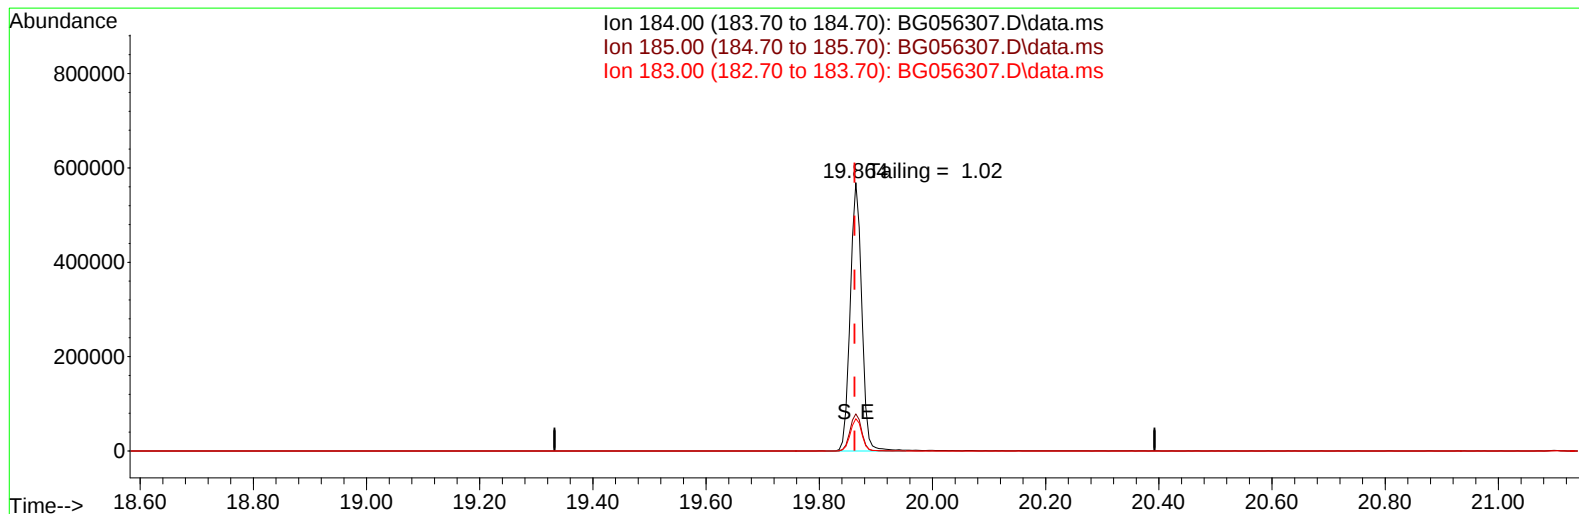

TIC: BG056307.D\data.ms

(77) Benzidine

19.864min (+ 0.002) 0.00 ng

response 807781

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	13.87
183.00	11.70	12.04
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/17/2023	BNA_G	<u>BG056307.D</u>
Compound Name	Response	Retention Time
DDT	388340	21.098
DDD	24140	20.646
DDE	3474	20.146
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
27614	415954	6.64

Instrument :
BNA_G
ClientSampleId :
DFTPP