
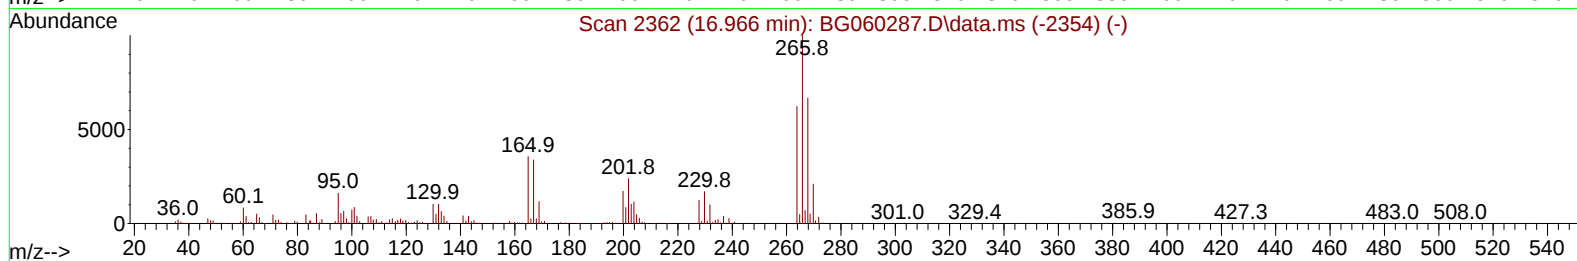
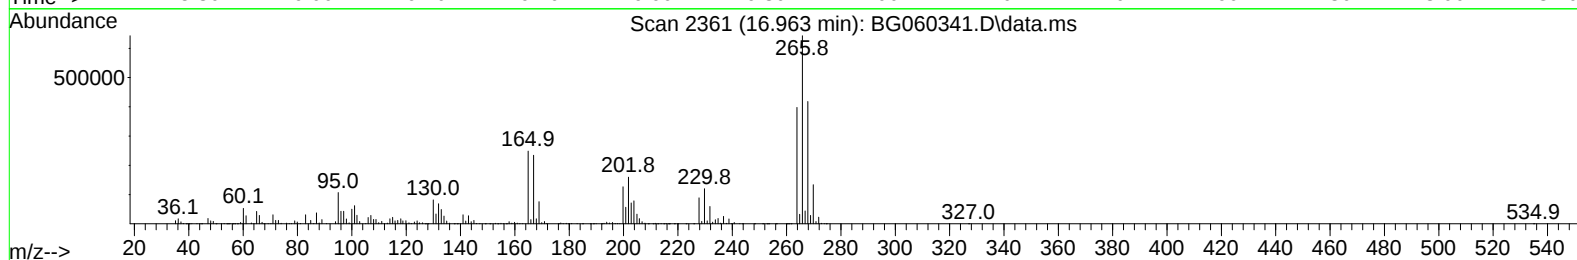


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011724\
Data File : BG060341.D
Acq On : 17 Jan 2024 12:59
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 17 13:47:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration

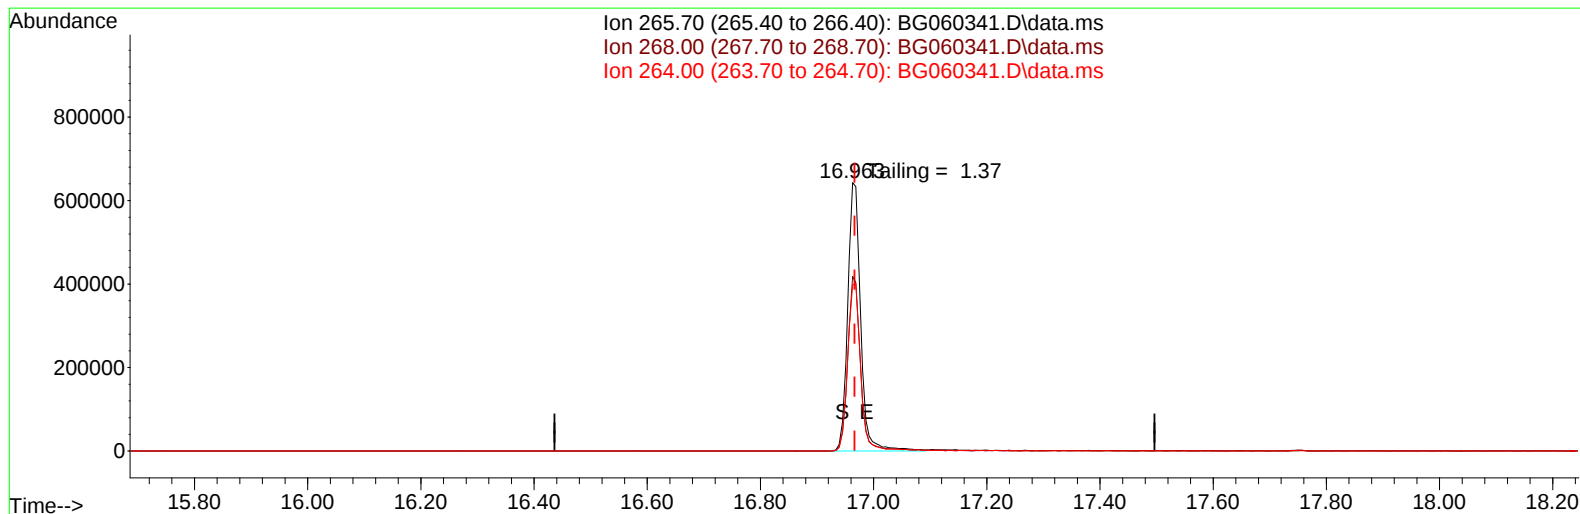

TIC: BG060341.D\data.ms

(70) Pentachlorophenol (C)




16.963min (-0.003) 705305.19 ng

response 1023569

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	71.80	65.07
264.00	62.30	61.89
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011724\
Data File : BG060341.D
Acq On : 17 Jan 2024 12:59
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 17 13:47:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration

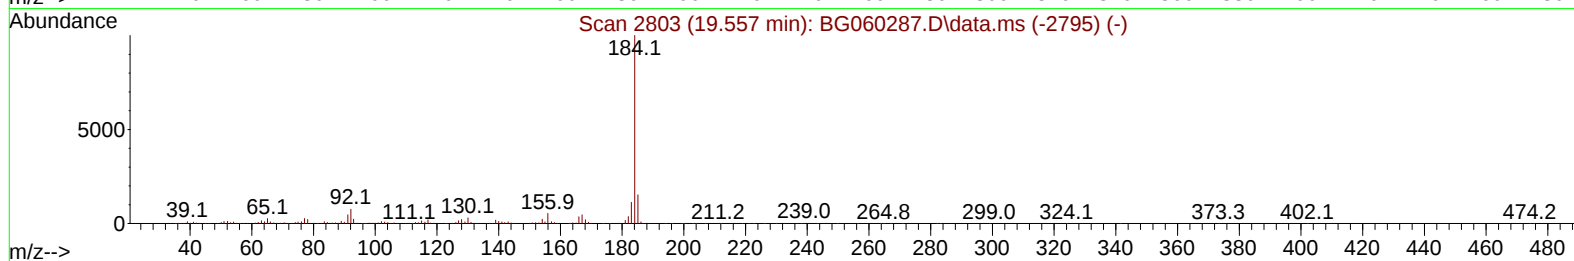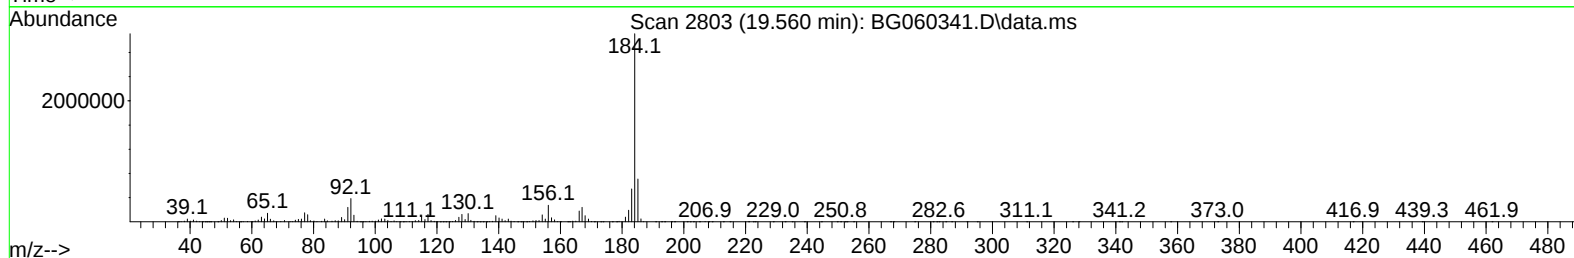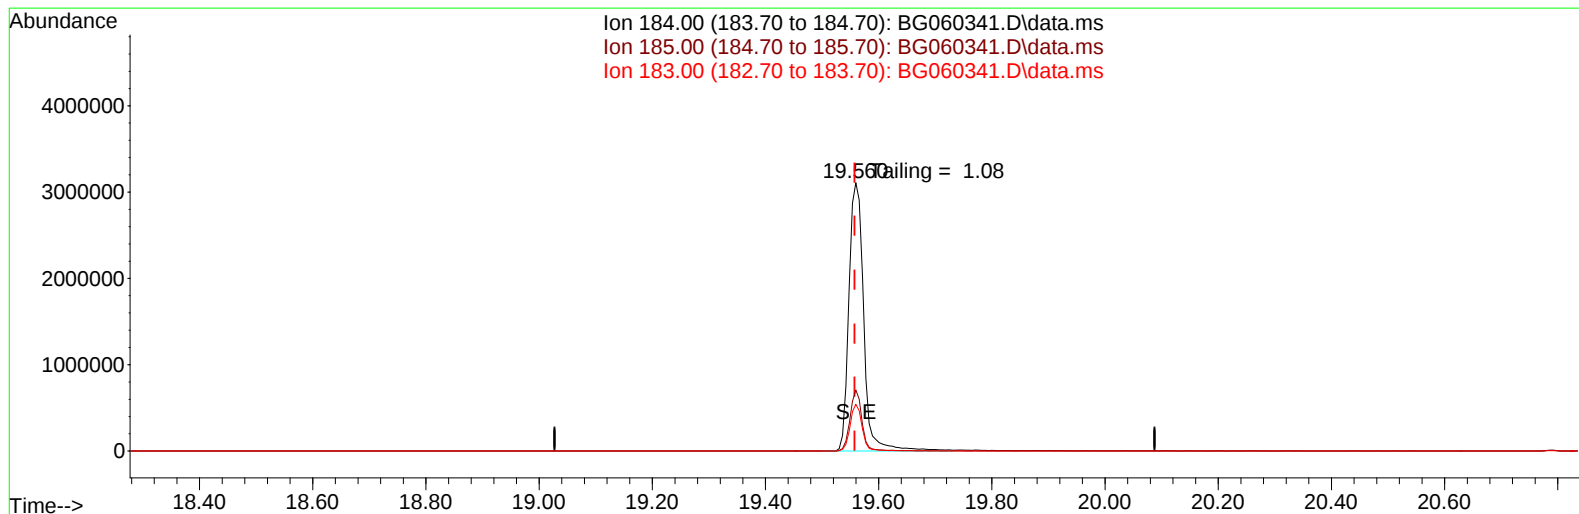

TIC: BG060341.D\data.ms

(77) Benzidine**19.560min (+ 0.003) 3379301.90 ng****response 5653034**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	22.71#
183.00	11.20	17.41#
0.00	0.00	0.00