


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011724\
Data File : BG060341.D
Acq On : 17 Jan 2024 12:59
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jan 09 04:07:12 2024

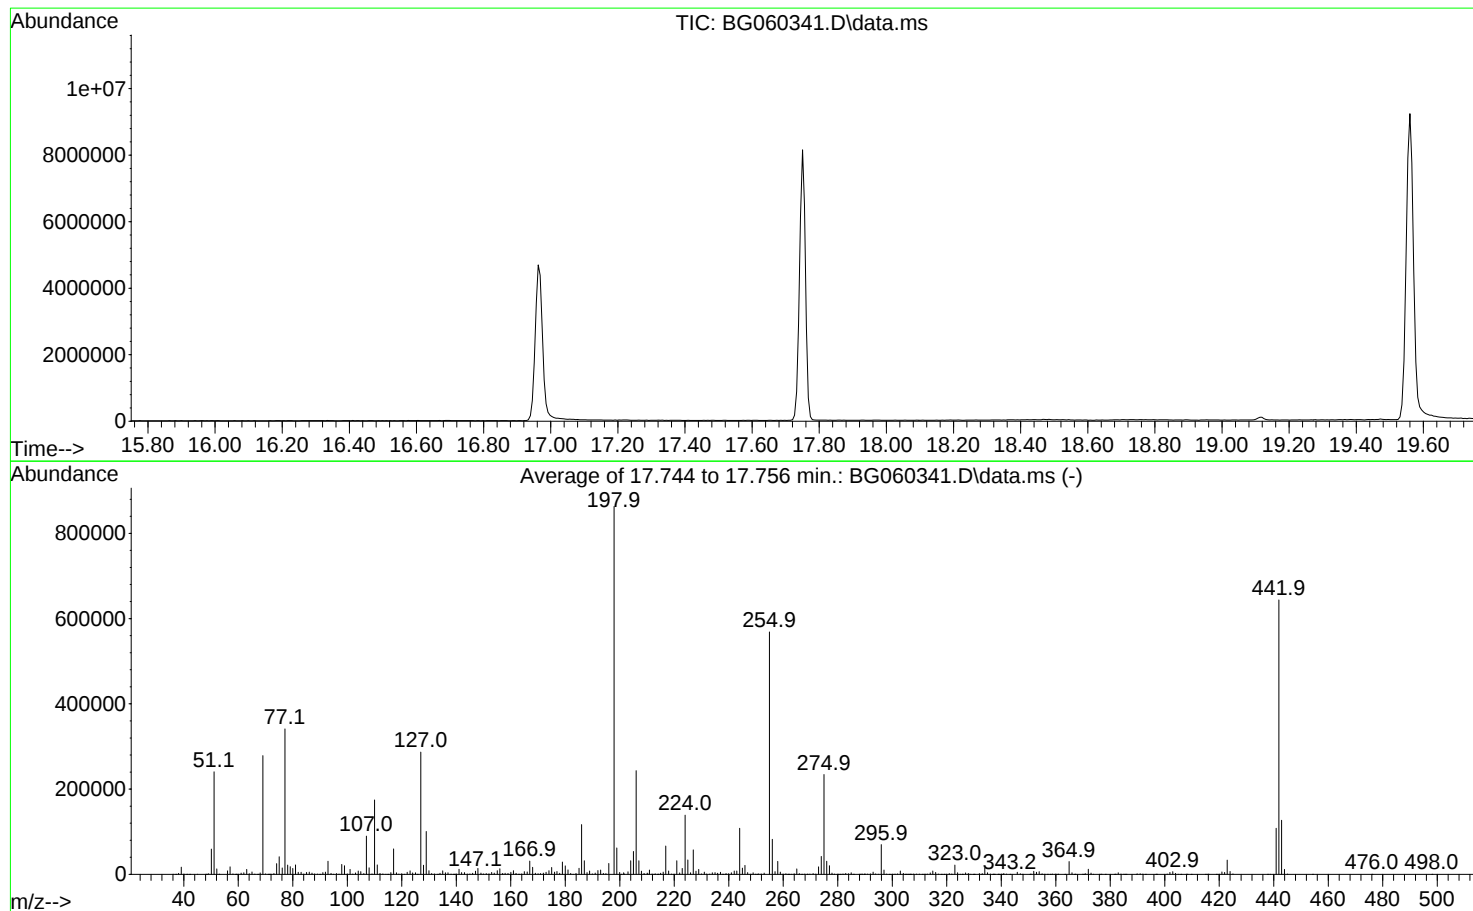




AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2486

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.9	240619	PASS
68	69	0.00	2	1.2	3317	PASS
69	198	0.00	100	32.3	278671	PASS
70	69	0.00	2	0.4	1051	PASS
127	198	10	80	33.2	286656	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	862997	PASS
199	198	5	9	7.2	61941	PASS
275	198	10	60	27.1	234176	PASS
365	198	1	100	3.5	30224	PASS
441	198	0.01	100	12.5	108069	PASS
442	442	50	100	100.0	643861	PASS
443	442	15	24	19.7	126880	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011724\
Data File : BG060341.D
Acq On : 17 Jan 2024 12:59
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 17 13:47:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration

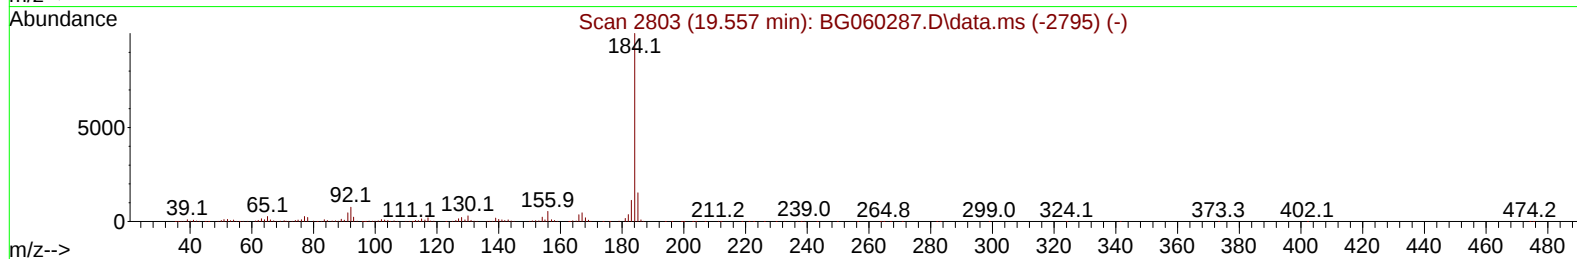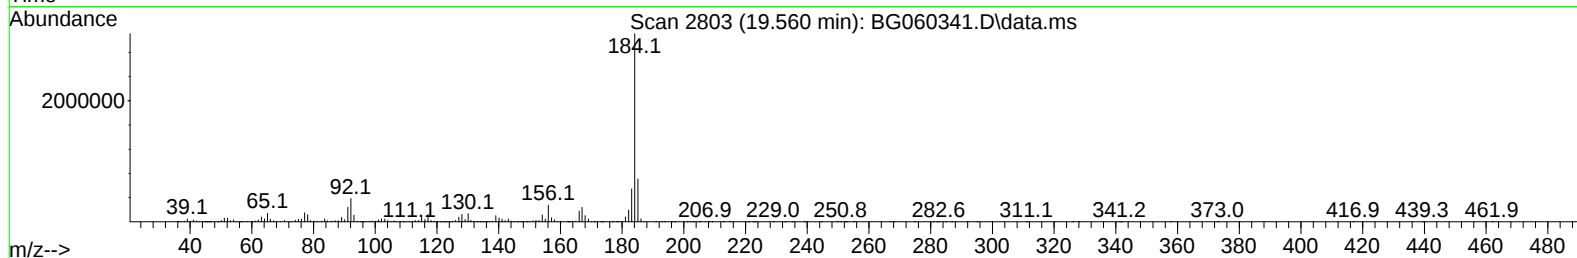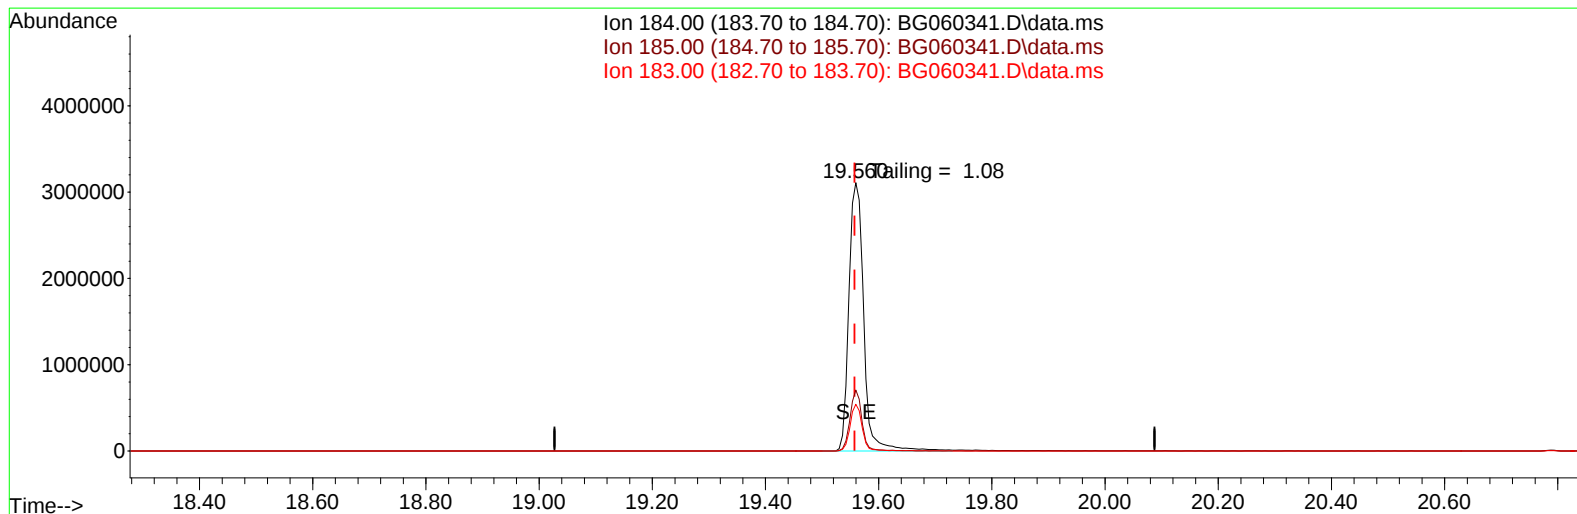

TIC: BG060341.D\data.ms

(77) Benzidine

19.560min (+ 0.003) 3379301.90 ng

response 5653034

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	22.71#
183.00	11.20	17.41#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/17/2024	BNA_G	<u>BG060341.D</u>
Compound Name	Response	Retention Time
DDT	2991356	20.788
DDD	59514	20.4
DDE	2194	19.836
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
61708	3053064	2.02

Instrument :
BNA_G
ClientSampleId :
DFTPP