
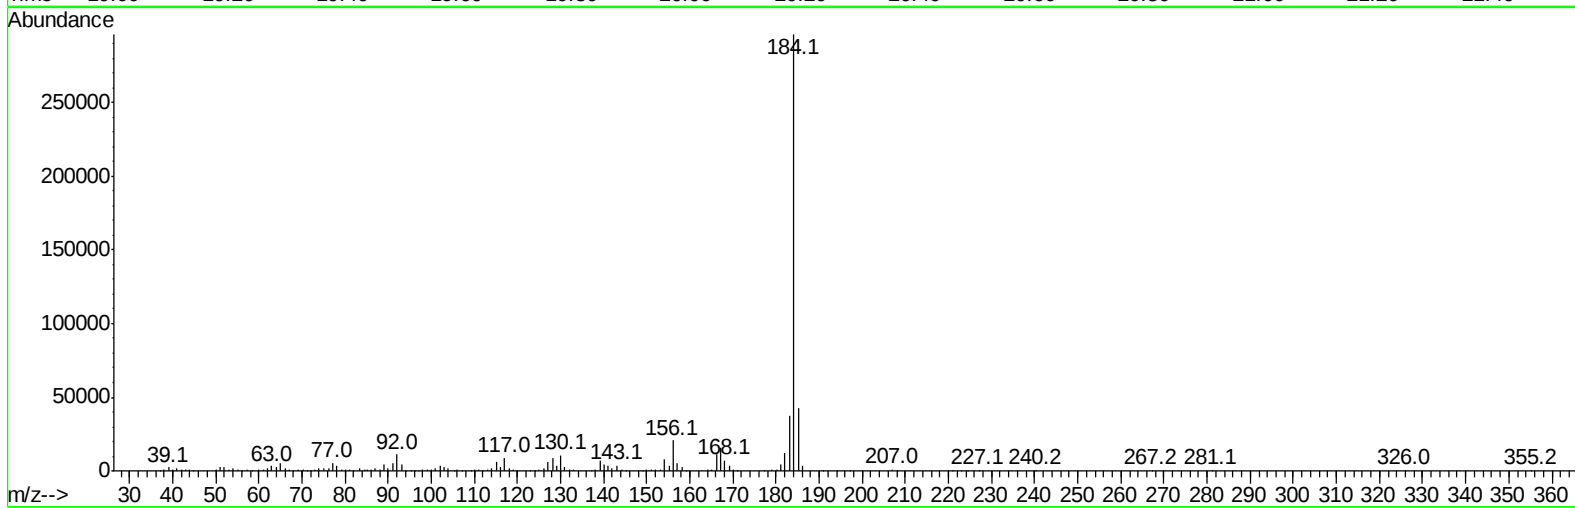


Data Path : U:\HPCHEM1\BNA G\DATA\BG011818\
Data File : BG032138.D
Acq On : 18 Jan 2018 16:23
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 19 06:07:40 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG011218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 18 10:13:16 2018
Response via : Initial Calibration

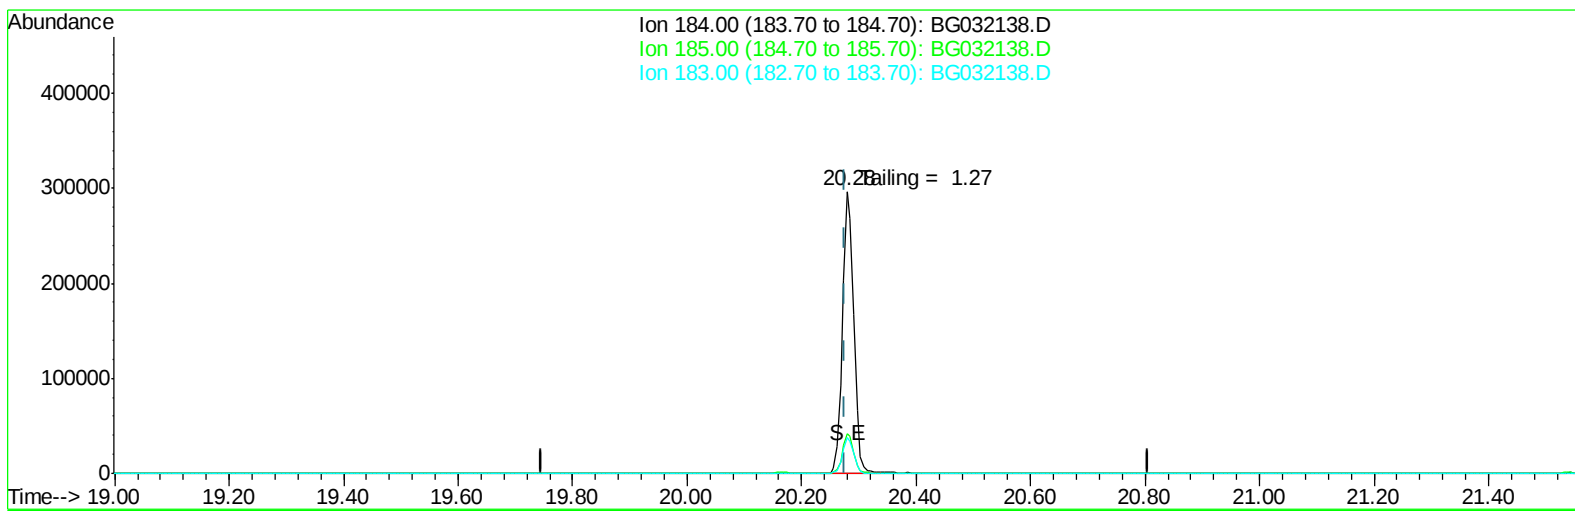

TIC: BG032138.D

(76) Benzidine



20.279min (+0.004) 254449.65ng

response 413583

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.33
183.00	13.30	12.55
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA G\DATA\BG011818\
Data File : BG032138.D
Acq On : 18 Jan 2018 16:23
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 19 06:07:40 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG011218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 18 10:13:16 2018
Response via : Initial Calibration

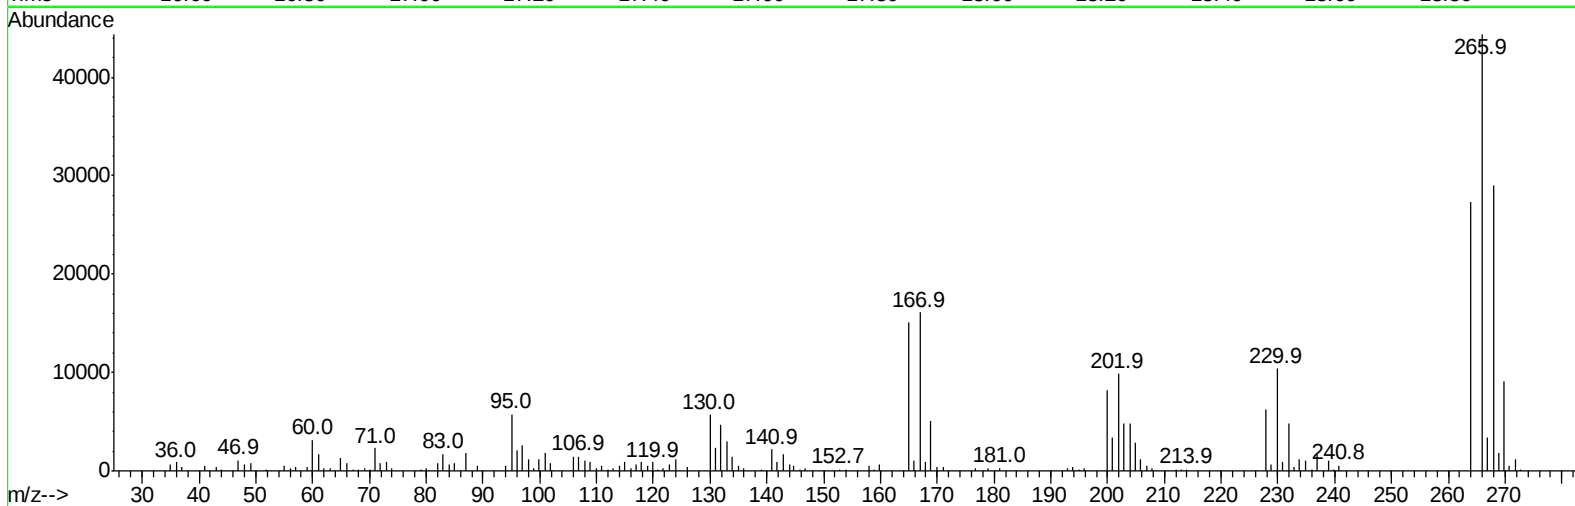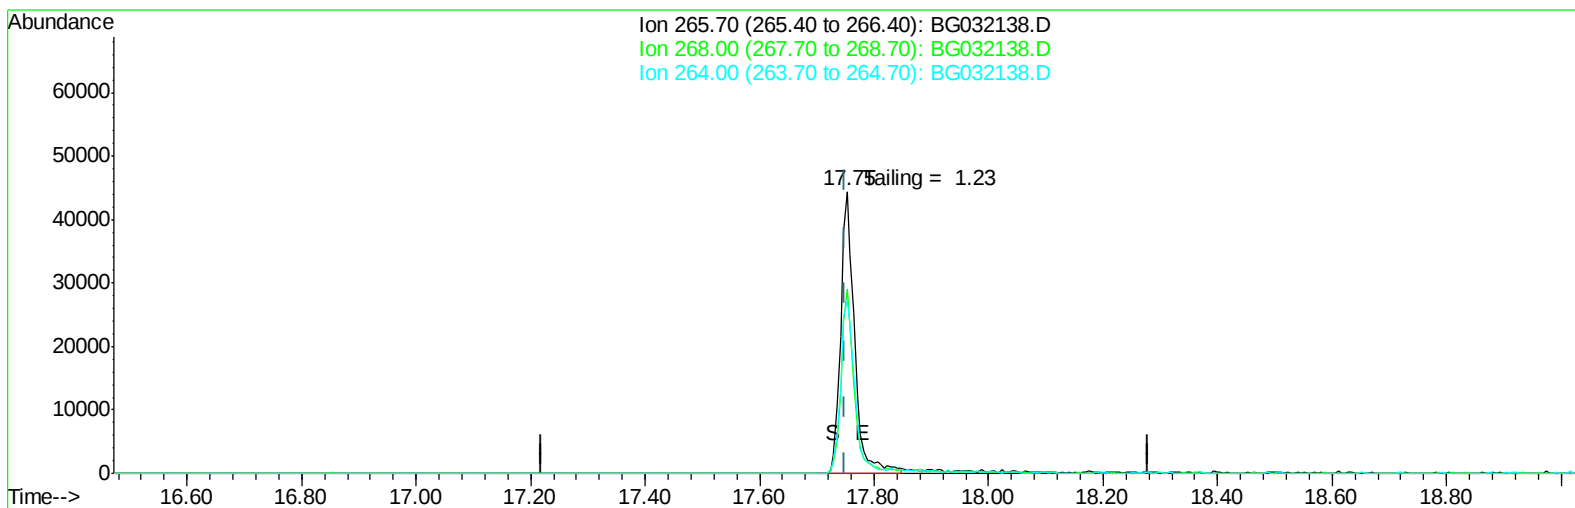

TIC: BG032138.D

(69) Pentachlorophenol (C)

17.753min (+0.004) 21084.47ng

response 73826

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	65.51
264.00	62.00	61.47
0.00	0.00	0.00