

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_G\DATA\BG011818\
 Data File : BG032148.D
 Acq On : 18 Jan 2018 22:39
 Operator : SJ/JU
 Sample : J1187-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 EPE-106-4A(37-39)

Quant Time: Jan 19 05:32:58 2018
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG011218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 18 10:13:16 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.75	152	38630	20.00	ng	0.00
21) Naphthalene-d8	11.62	136	167313	20.00	ng	0.00
38) Acenaphthene-d10	15.38	164	123751	20.00	ng	0.00
63) Phenanthrene-d10	18.11	188	347435	20.00	ng	0.00
75) Chrysene-d12	22.45	240	456464	20.00	ng	0.00
86) Perylene-d12	26.14	264	461513	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	6.17	112	240315	113.78	ng	0.00
7) Phenol-d6	7.85	99	320243	120.39	ng	0.00
23) Nitrobenzene-d5	9.94	82	190974	77.22	ng	0.00
41) 2,4,6-Tribromophenol	16.85	330	249919	122.04	ng	0.00
44) 2-Fluorobiphenyl	14.00	172	679565	68.09	ng	0.00
78) Terphenyl-d14	20.65	244	1390150	67.25	ng	0.00
Target Compounds						
10) Phenol	7.88	94	12502	4.771	ng	Qvalue 93
49) Dimethylphthalate	14.80	163	96677	8.927	ng	# 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_G\DATA\BG011818\
Data File : BG032148.D
Acq On : 18 Jan 2018 22:39
Operator : SJ/JU
Sample : J1187-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
EPE-106-4A(37-39)

Quant Time: Jan 19 05:32:58 2018
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG011218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 18 10:13:16 2018
Response via : Initial Calibration

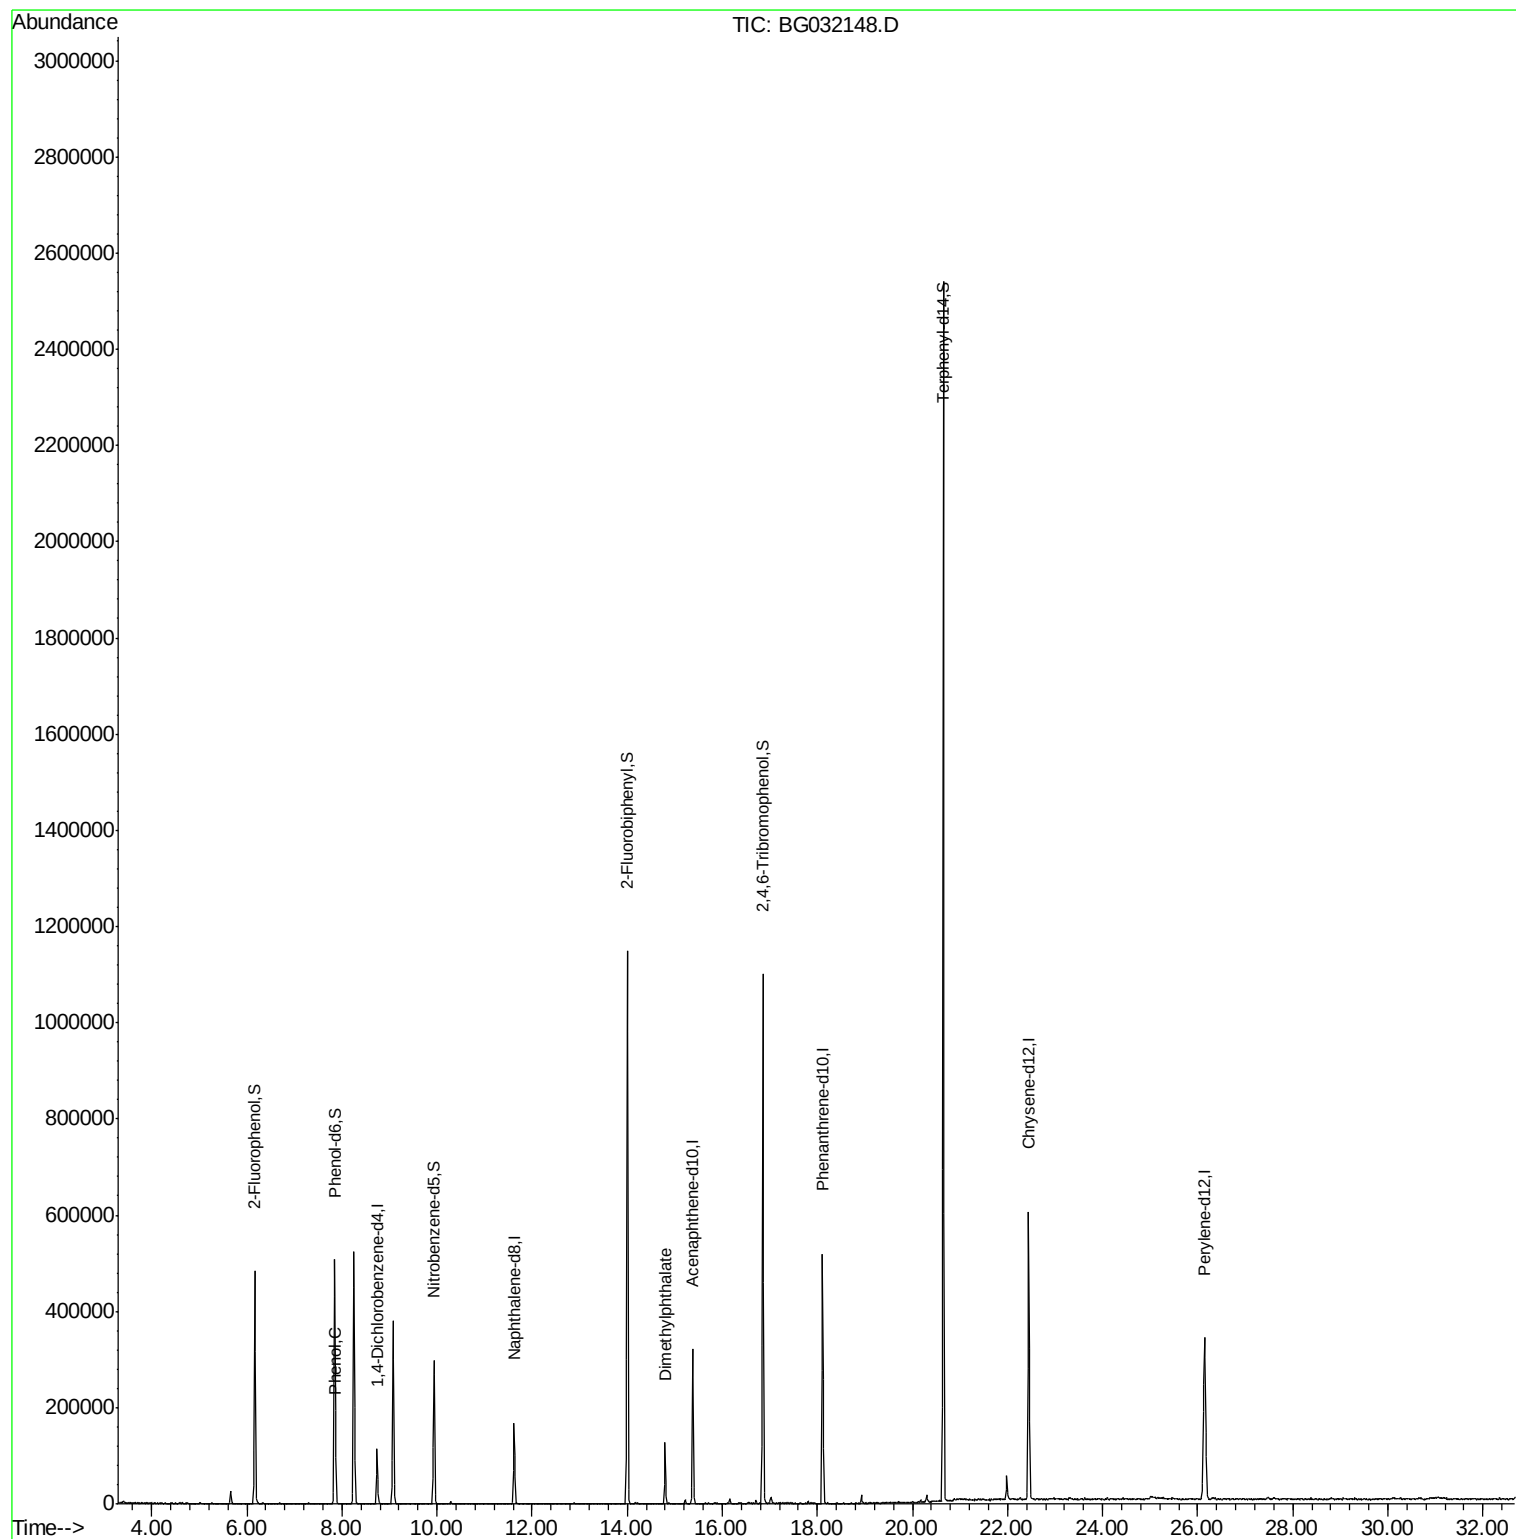




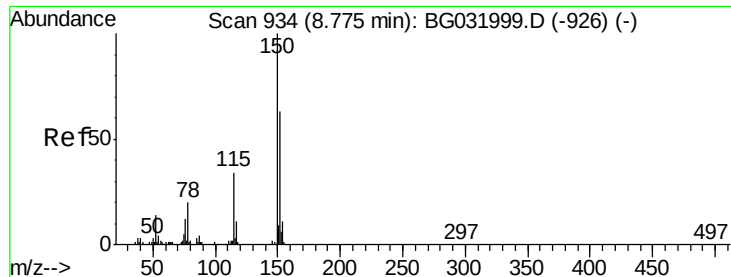


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.75 min Scan# 929
Delta R.T. 0.00 min
Lab File: BG032148.D
Acq: 18 Jan 2018 22:39

Instrument :
BNA_G
ClientSampleId :
EPE-106-4A(37-39)




Tgt Ion:152 Resp: 38630
Ion Ratio Lower Upper
152 100
150 138.6 126.6 189.8
115 47.5 53.0 79.4#

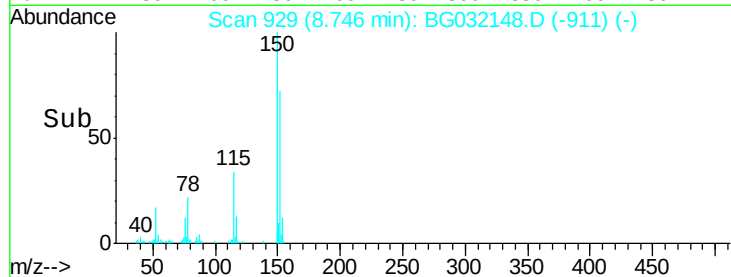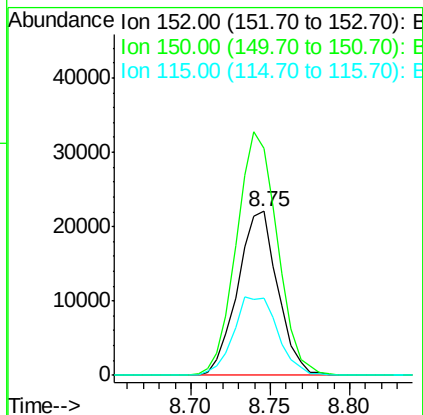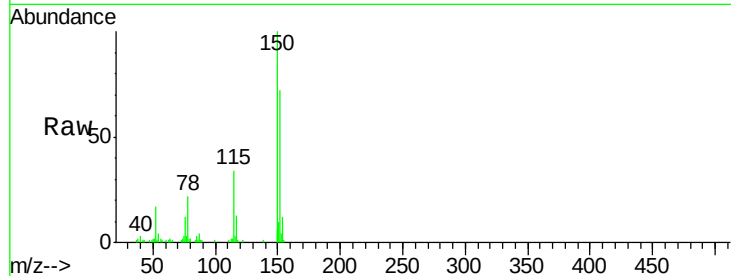


#5

2-Fluorophenol
Concen: 113.777 ng
RT: 6.17 min Scan# 490
Delta R.T. -0.00 min
Lab File: BG032148.D
Acq: 18 Jan 2018 22:39

Tgt Ion:112 Resp: 240315
Ion Ratio Lower Upper
112 100
64 50.9 56.3 84.5#
63 30.1 30.1 45.1#

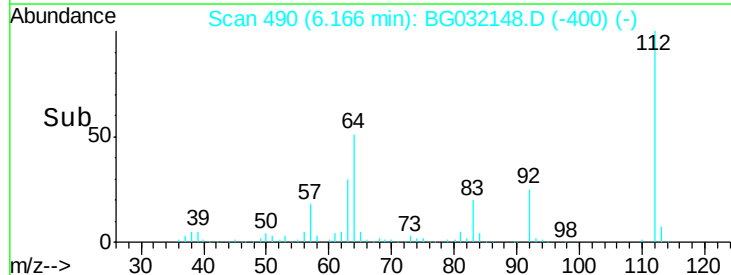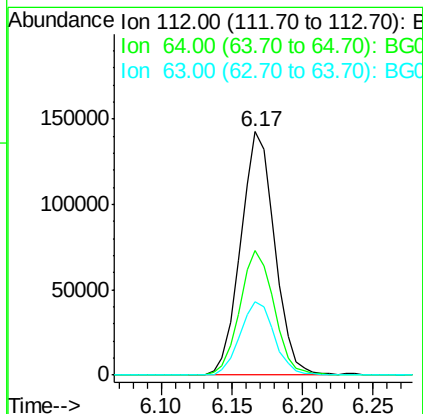

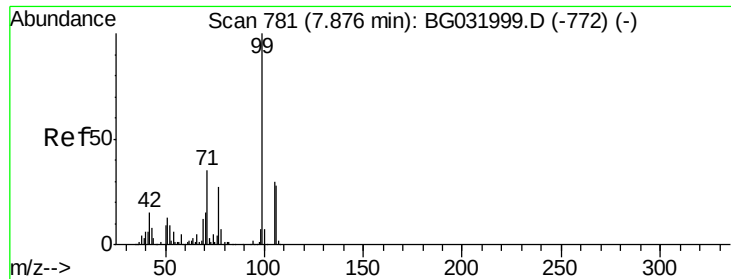

#7

Phenol-d6

Concen: 120.386 ng

RT: 7.85 min Scan# 776

Delta R.T. -0.00 min

Lab File: BG032148.D

Acq: 18 Jan 2018 22:39

Instrument :

BNA_G

ClientSampleId :

EPE-106-4A(37-39)


Tgt Ion: 99 Resp: 320243

Ion Ratio Lower Upper




99 100

42 17.2 14.1 21.1

71 40.5 26.1 39.1#

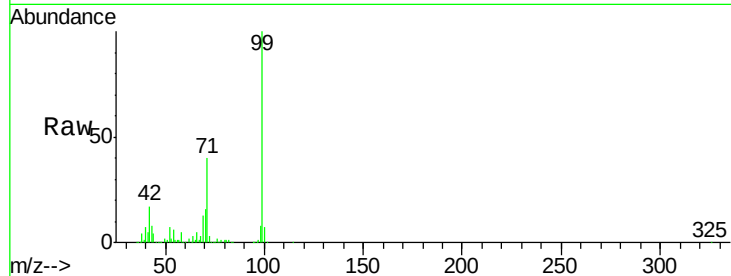

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

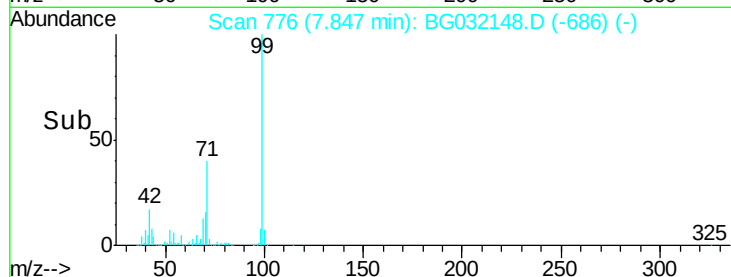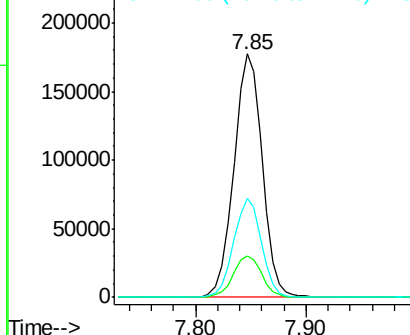

#10

Phenol

Concen: 4.771 ng

RT: 7.88 min Scan# 781

Delta R.T. -0.00 min

Lab File: BG032148.D

Acq: 18 Jan 2018 22:39


Tgt Ion: 94 Resp: 12502

Ion Ratio Lower Upper



94 100


65 28.9 11.9 51.9

66 47.6 22.2 62.2



Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC

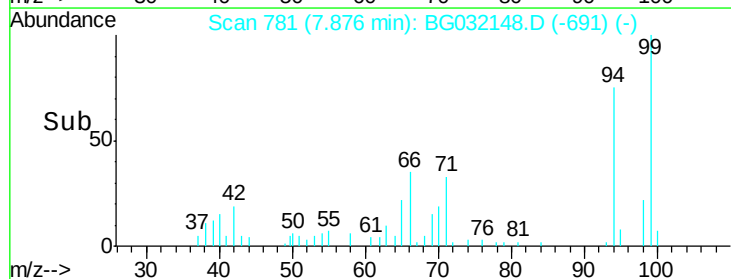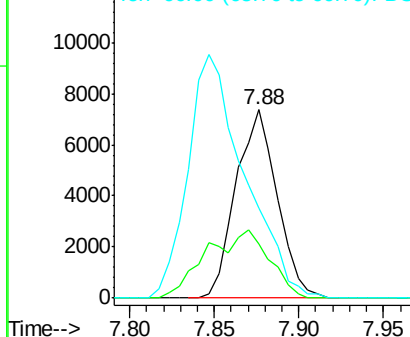

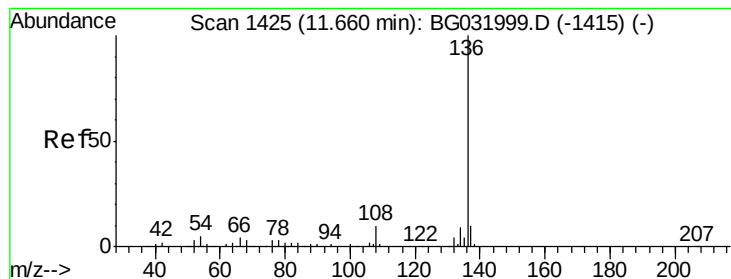

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 11.62 min Scan# 1419

Delta R.T. -0.00 min

Lab File: BG032148.D

Acq: 18 Jan 2018 22:39

Instrument :

BNA_G

ClientSampleId :

EPE-106-4A(37-39)

Tgt Ion:136 Resp: 167313


Ion Ratio Lower Upper

136 100

137 10.2 9.2 13.8

54 5.1 10.3 15.5#

68 3.3 4.5 6.7#






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BGC

Ion 68.00 (67.70 to 68.70): BGC

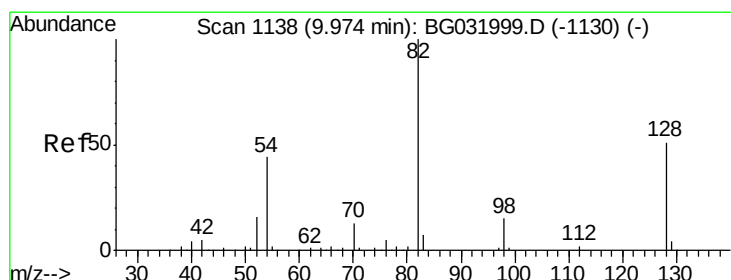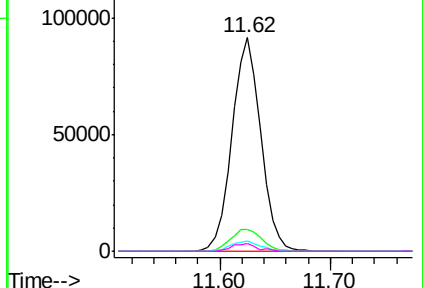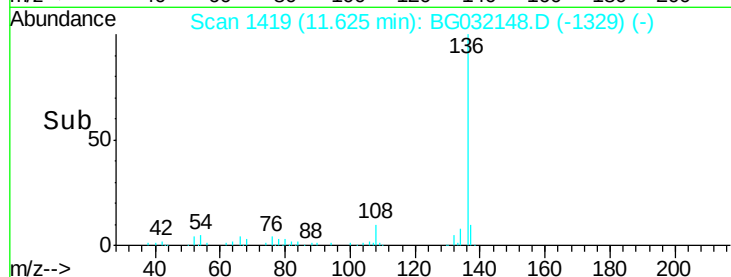

#23

Nitrobenzene-d5

Concen: 77.222 ng

RT: 9.94 min Scan# 1132

Delta R.T. -0.00 min

Lab File: BG032148.D

Acq: 18 Jan 2018 22:39


Tgt Ion: 82 Resp: 190974

Ion Ratio Lower Upper

82 100

128 48.4 29.7 44.5#



54 44.4 43.1 64.7




Abundance Ion 82.00 (81.70 to 82.70): BGC

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BGC

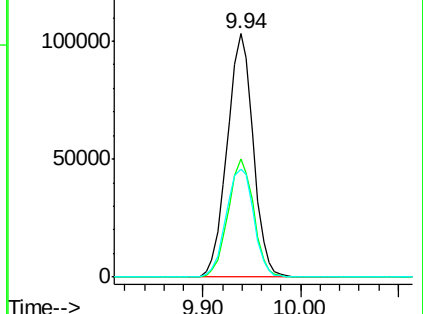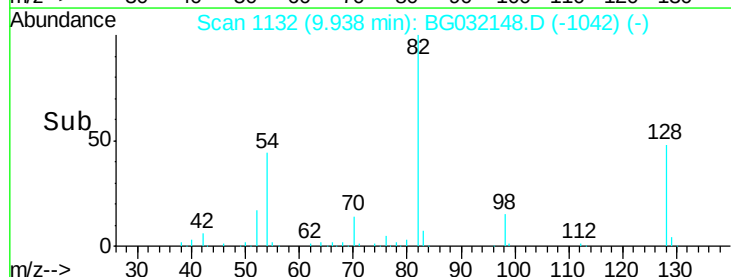

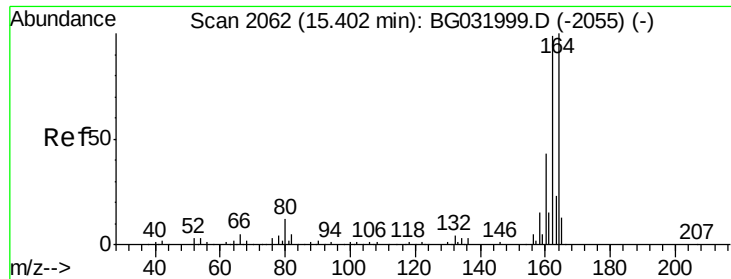

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 15.38 min Scan# 2058

Delta R.T. -0.00 min

Lab File: BG032148.D

Acq: 18 Jan 2018 22:39

Instrument :

BNA_G

ClientSampleId :

EPE-106-4A(37-39)


Tgt Ion:164 Resp: 123751

Ion Ratio Lower Upper

164 100

162 106.6 78.8 118.2




160 46.3 35.4 53.0



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

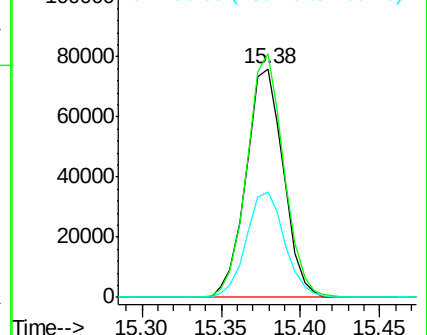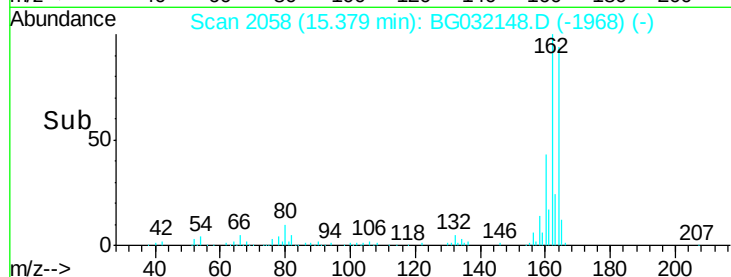

#41

2,4,6-Tribromophenol

Concen: 122.043 ng

RT: 16.85 min Scan# 2309

Delta R.T. -0.00 min

Lab File: BG032148.D

Acq: 18 Jan 2018 22:39


Tgt Ion:330 Resp: 249919

Ion Ratio Lower Upper

330 100

332 95.5 77.0 115.6



141 29.0 25.2 37.8




Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



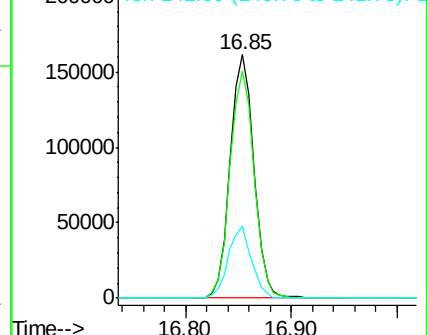
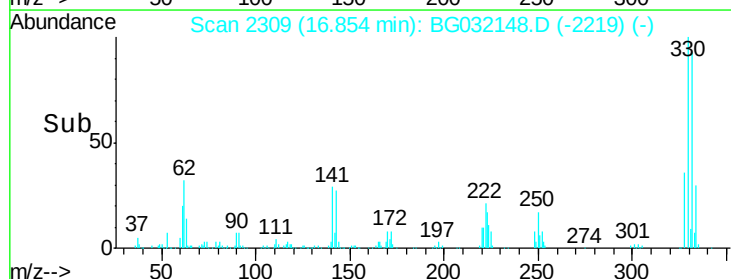


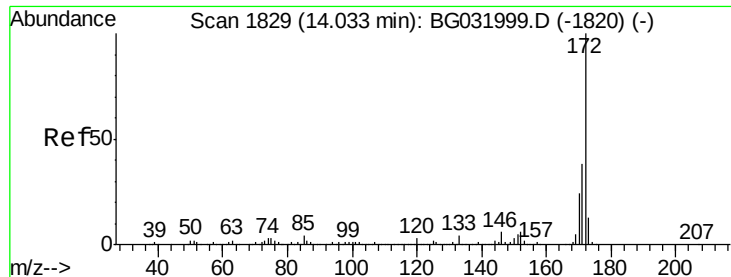

#44
2-Fluorobiphenyl
Concen: 68.091 ng
RT: 14.00 min Scan# 1824
Delta R.T. -0.00 min
Lab File: BG032148.D
Acq: 18 Jan 2018 22:39




Instrument :
BNA_G
ClientSampleId :
EPE-106-4A(37-39)


Tgt Ion:172 Resp: 679565
Ion Ratio Lower Upper
172 100
171 38.5 30.0 45.0
170 22.7 19.5 29.3

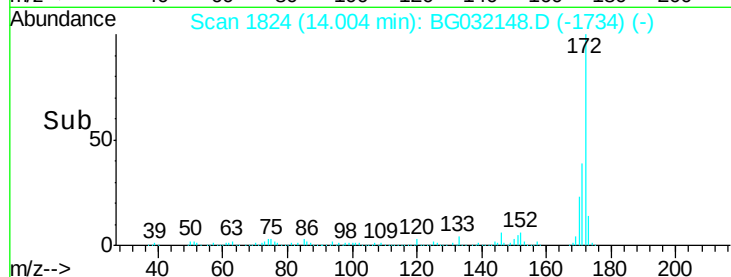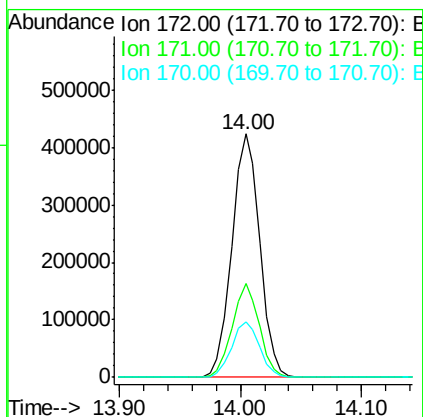

#49
Dimethylphthalate
Concen: 8.927 ng
RT: 14.80 min Scan# 1960
Delta R.T. -0.01 min
Lab File: BG032148.D
Acq: 18 Jan 2018 22:39

Tgt Ion:163 Resp: 96677
Ion Ratio Lower Upper
163 100
194 5.4 3.4 5.2#
164 9.3 8.2 12.4

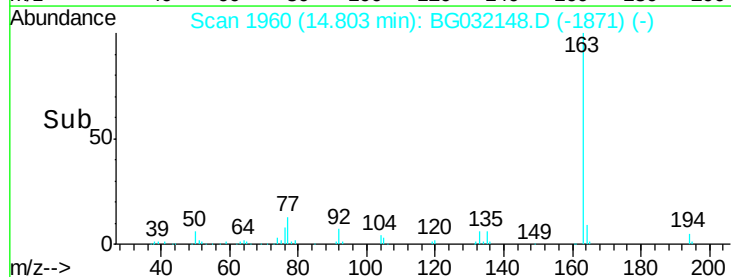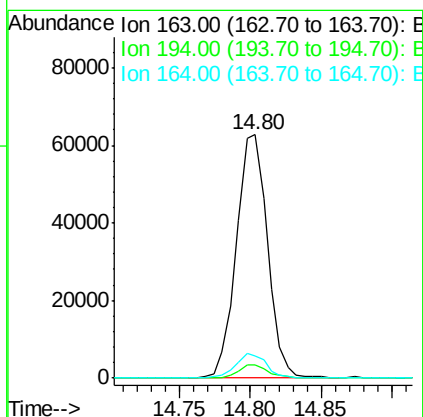


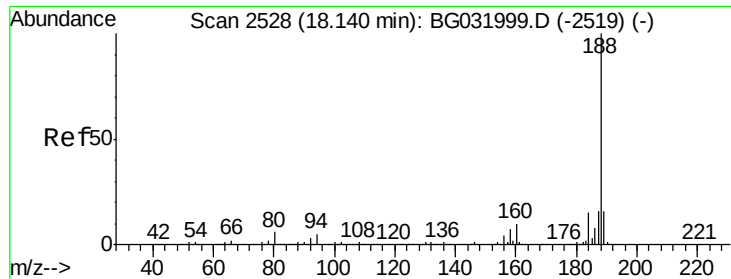




#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 18.11 min Scan# 2523
Delta R.T. -0.00 min
Lab File: BG032148.D
Acq: 18 Jan 2018 22:39

Instrument :
BNA_G
ClientSampleId :
EPE-106-4A(37-39)

Tgt Ion:188 Resp: 347435
Ion Ratio Lower Upper
188 100
94 4.7 6.9 10.3#
80 4.7 7.7 11.5#




Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC

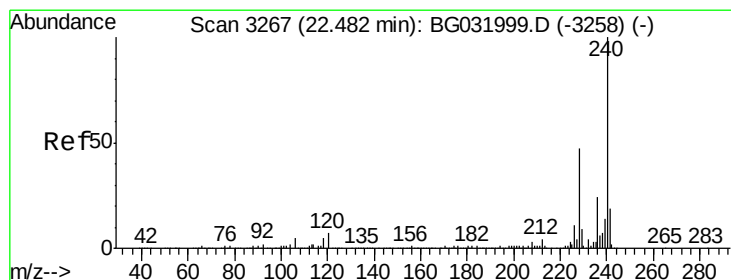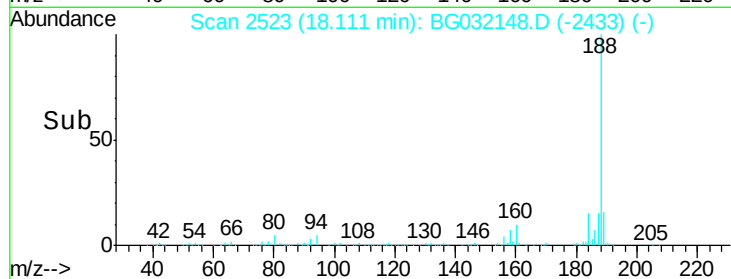
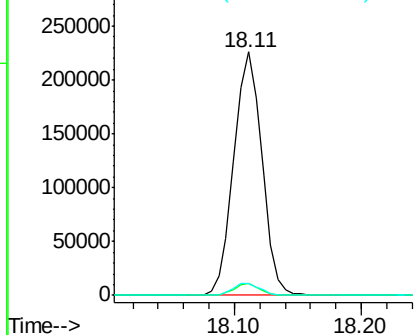



#75
Chrysene-d12
Concen: 20.000 ng
RT: 22.45 min Scan# 3261
Delta R.T. -0.00 min
Lab File: BG032148.D
Acq: 18 Jan 2018 22:39

Tgt Ion:240 Resp: 456464
Ion Ratio Lower Upper
240 100
120 4.7 6.8 10.2#
236 26.2 20.9 31.3

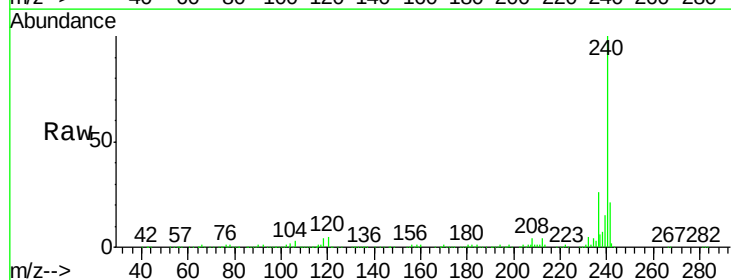

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

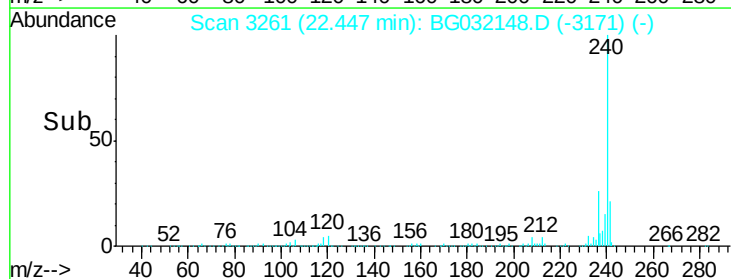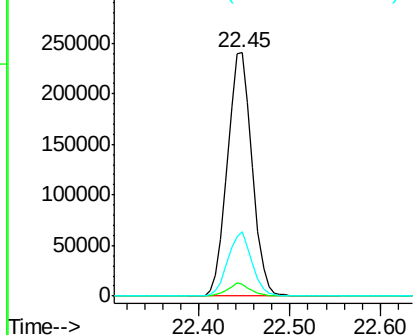

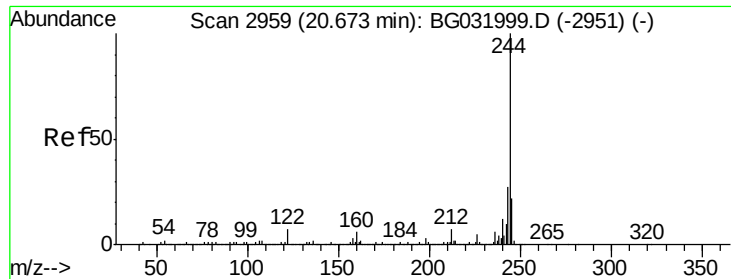

#78

Terphenyl-d14

Concen: 67.245 ng

RT: 20.65 min Scan# 2955

Delta R.T. -0.00 min

Lab File: BG032148.D

Acq: 18 Jan 2018 22:39

Instrument :

BNA_G

ClientSampleId :

EPE-106-4A(37-39)


Tgt Ion:244 Resp: 1390150

Ion Ratio Lower Upper

244 100

212 7.7 5.8 8.8




122 5.9 7.0 10.4#

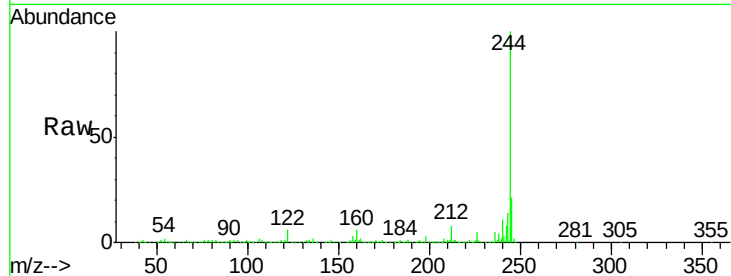

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

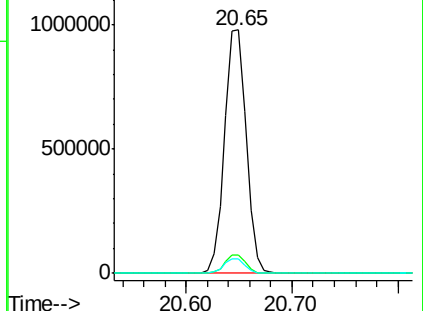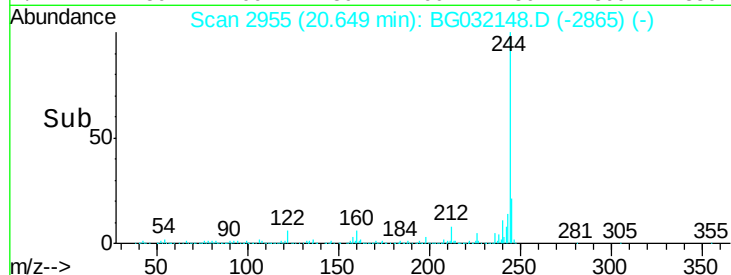

#86

Perylene-d12

Concen: 20.000 ng

RT: 26.14 min Scan# 3890

Delta R.T. -0.01 min

Lab File: BG032148.D

Acq: 18 Jan 2018 22:39


Tgt Ion:264 Resp: 461513

Ion Ratio Lower Upper

264 100

260 25.0 17.4 26.0

265 22.3 17.7 26.5



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

