
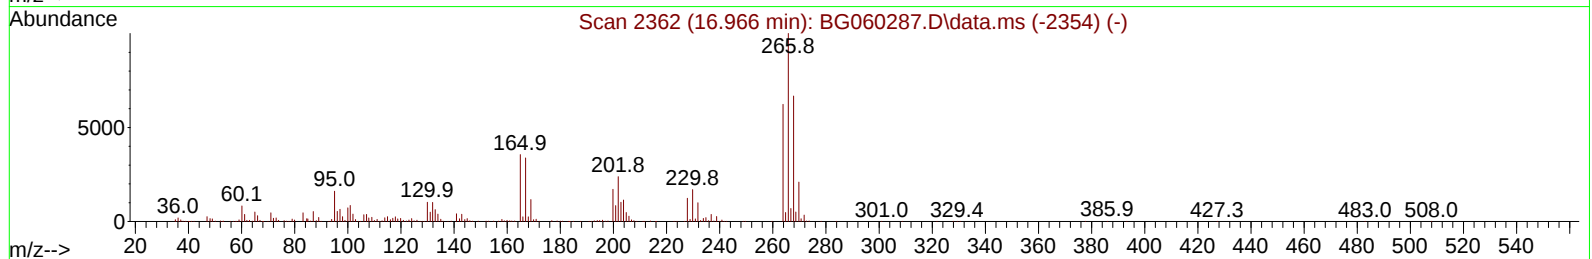
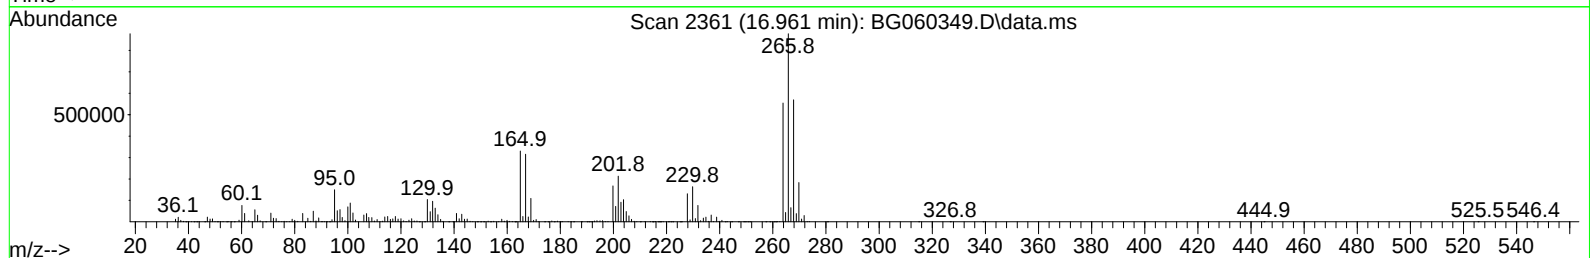


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011824\
Data File : BG060349.D
Acq On : 18 Jan 2024 12:42
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 18 13:29:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration

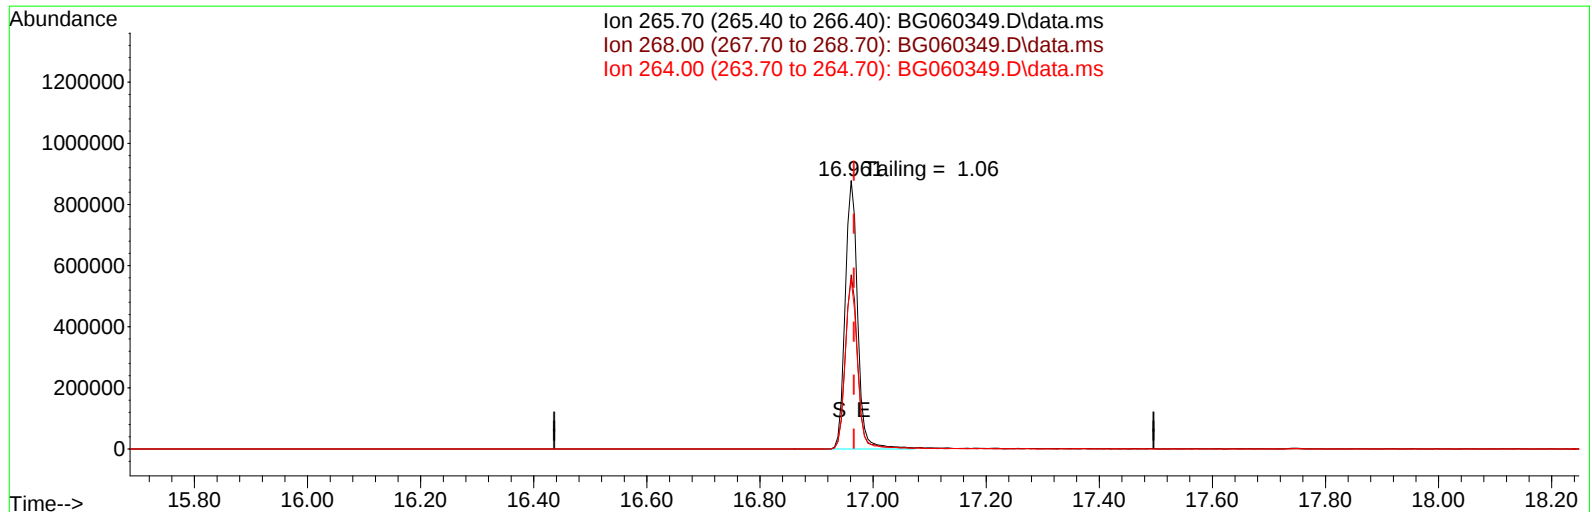

TIC: BG060349.D\data.ms

(70) Pentachlorophenol (C)




16.961min (-0.005) 1425625.23 ng

response 1349301

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	71.80	64.85
264.00	62.30	63.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011824\
Data File : BG060349.D
Acq On : 18 Jan 2024 12:42
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 18 13:29:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration

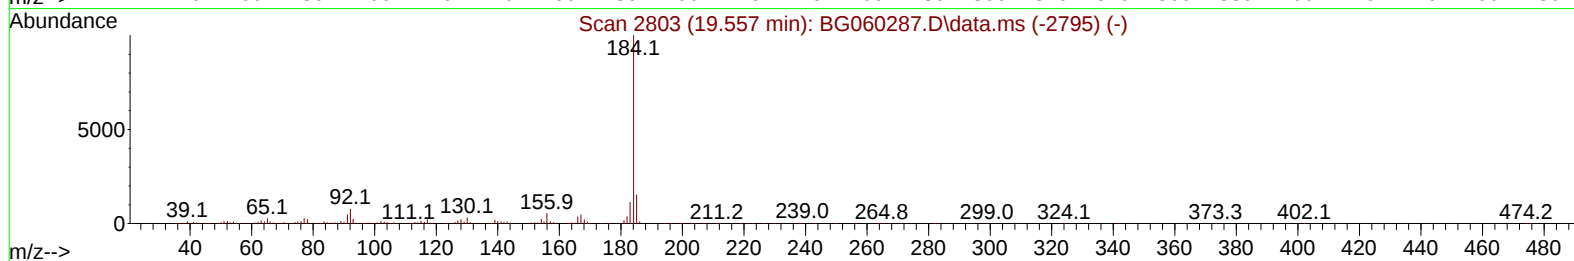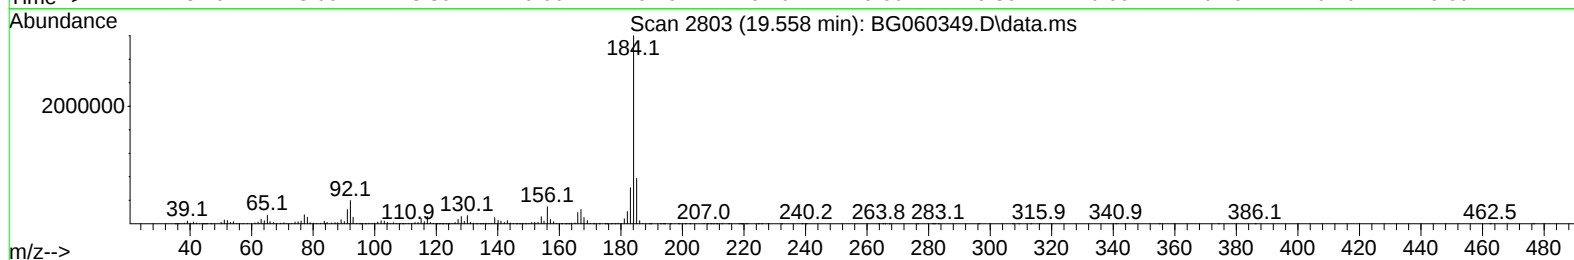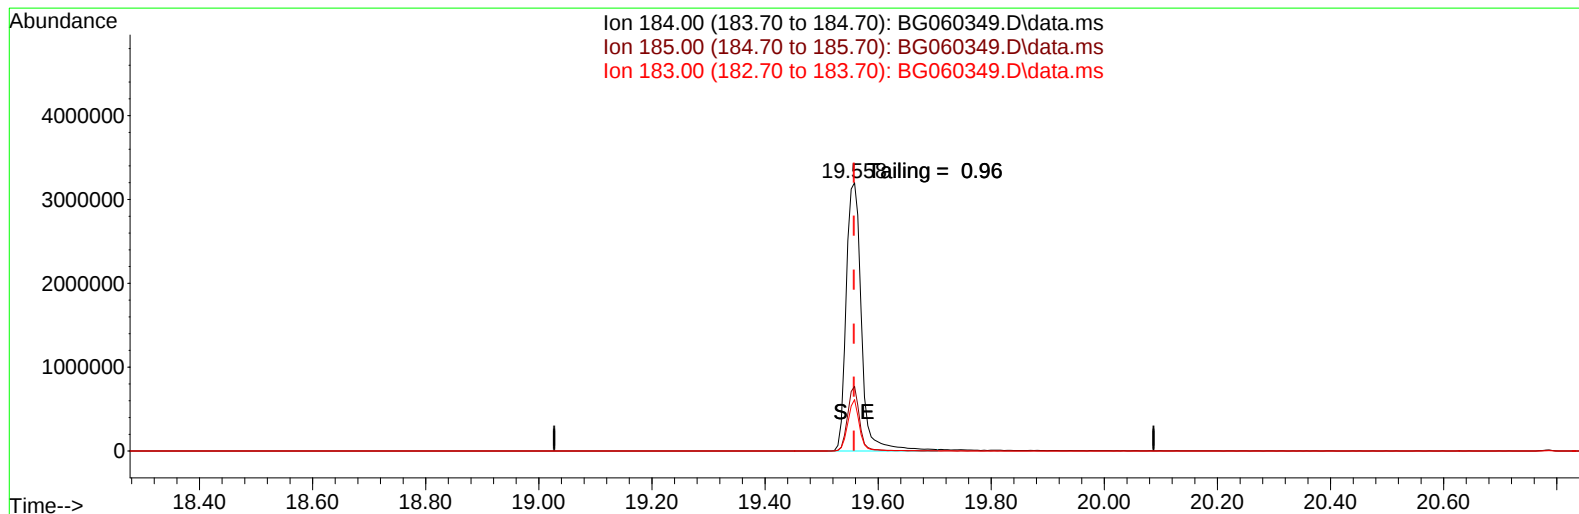

TIC: BG060349.D\data.ms

(77) Benzidine

19.558min (+ 0.001) 4023782.88 ng

response 6031808

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	24.12#
183.00	11.20	19.17#
0.00	0.00	0.00