

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011824\
 Data File : BG060355.D
 Acq On : 18 Jan 2024 16:50
 Operator : MA/JU
 Sample : P1159-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 TP-011724

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG060355.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.500	404	410	426	rBV	3472226	5711513	42.74%	8.751%
2	7.092	674	681	702	rBV	3621764	6314493	47.25%	9.674%
3	7.926	816	823	831	rBV	865325	1460621	10.93%	2.238%
4	9.090	1012	1021	1033	rBV	1859194	3406906	25.49%	5.220%
5	10.729	1293	1300	1313	rBV	1026363	1887371	14.12%	2.892%
6	13.185	1708	1718	1732	rBV	5775018	9151743	68.48%	14.021%
7	14.566	1944	1953	1960	rBV	1843012	2928396	21.91%	4.487%
8	16.052	2199	2206	2219	rBV	4164213	6568569	49.15%	10.064%
9	17.310	2414	2420	2427	rBV	2482408	3792187	28.38%	5.810%
10	18.197	2567	2571	2576	rBV4	111534	210493	1.58%	0.322%
11	19.366	2767	2770	2776	rVB	103093	145644	1.09%	0.223%
12	19.930	2860	2866	2875	rBV	10237223	13364415	100.00%	20.476%
13	21.217	3081	3085	3097	rVB2	330623	561355	4.20%	0.860%
14	21.569	3139	3145	3162	rVB	2476137	4295452	32.14%	6.581%
15	21.757	3174	3177	3182	rVB5	130079	178717	1.34%	0.274%
16	22.357	3275	3279	3285	rVB2	125218	196365	1.47%	0.301%
17	23.032	3389	3394	3404	rBV2	143088	302711	2.27%	0.464%
18	23.820	3524	3528	3536	rVB4	137898	275959	2.06%	0.423%
19	24.736	3674	3684	3703	rBV2	1405142	4516765	33.80%	6.920%




Sum of corrected areas: 65269675

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011824\
Data File : BG060355.D
Acq On : 18 Jan 2024 16:50
Operator : MA/JU
Sample : P1159-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-011724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

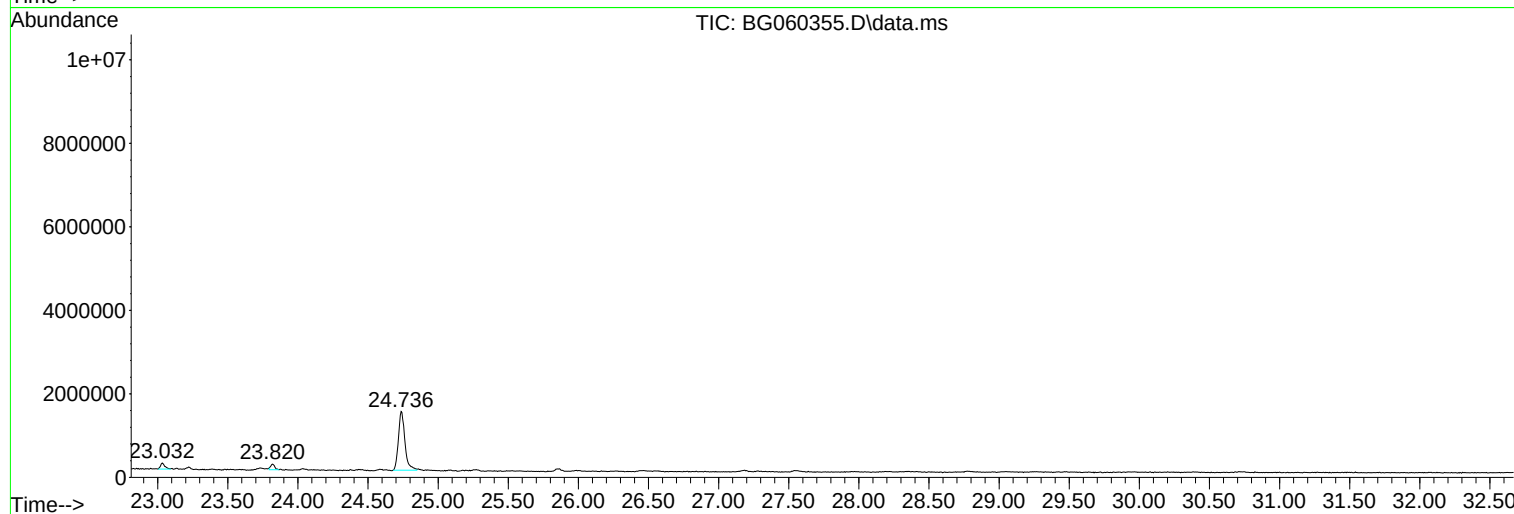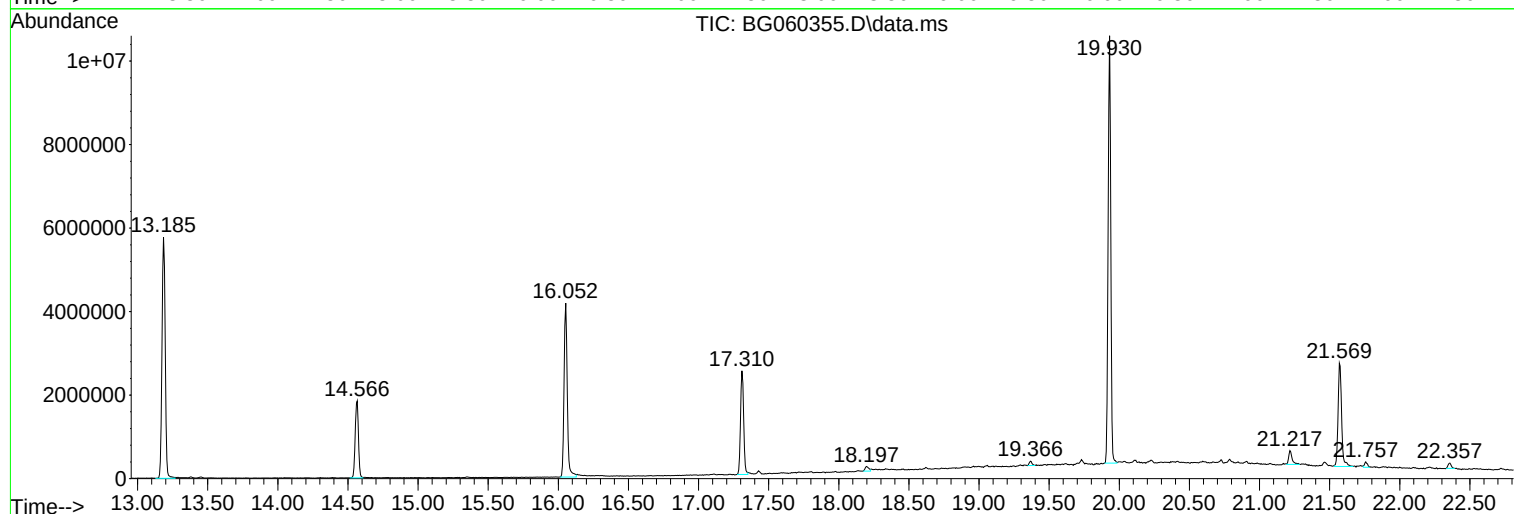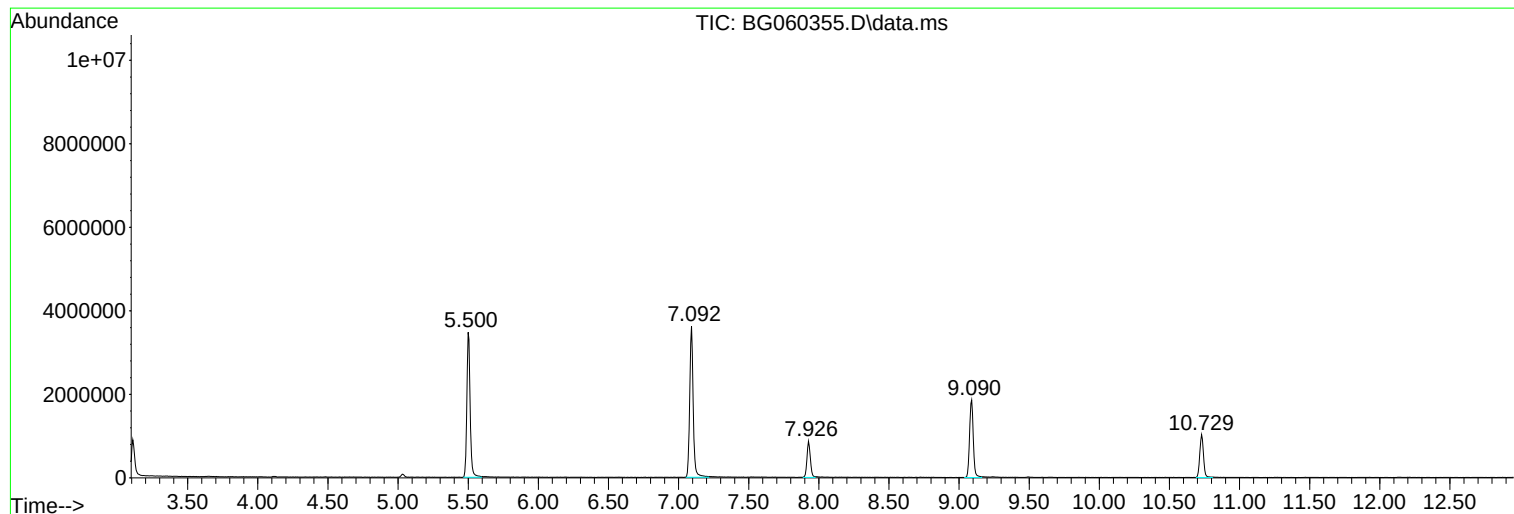

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011824\
Data File : BG060355.D
Acq On : 18 Jan 2024 16:50
Operator : MA/JU
Sample : P1159-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-011724










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Nonadecyl pentafluoropropio... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.217	2.61 ng	561355	Chrysene-d12	21.569

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Nonadecyl pentafluoropropionate	430	C22H39F5O2	1000351-88-8	91
2			Nonadecyl trifluoroacetate	380	C21H39F3O2	1000351-76-3	90
3			1-Hexacosanol	382	C26H54O	000506-52-5	90
4			Oxalic acid, octadecyl propyl ester	384	C23H44O4	1000309-27-0	80
5			Dichloroacetic acid, heptadecyl ...	366	C19H36Cl2O2	1000282-98-2	72

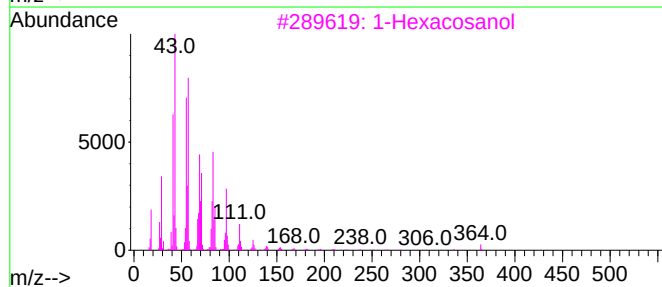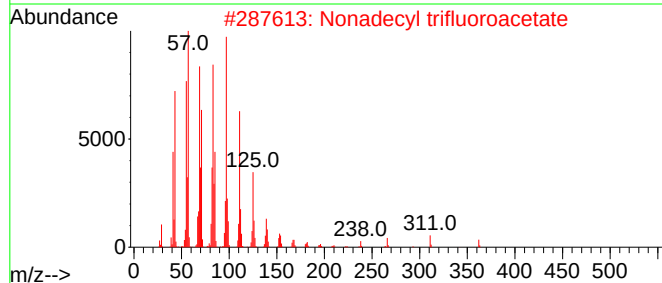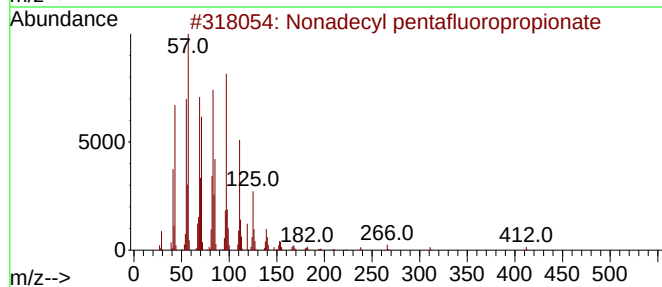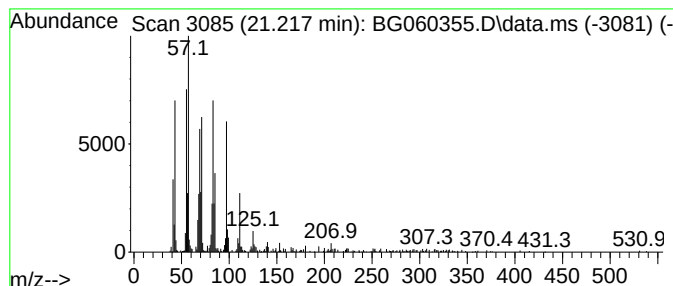

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011824\
Data File : BG060355.D
Acq On : 18 Jan 2024 16:50
Operator : MA/JU
Sample : P1159-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-011724

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Nonadecyl penta...	21.217	2.6	ng	561355	5	21.569	4295450	20.0