
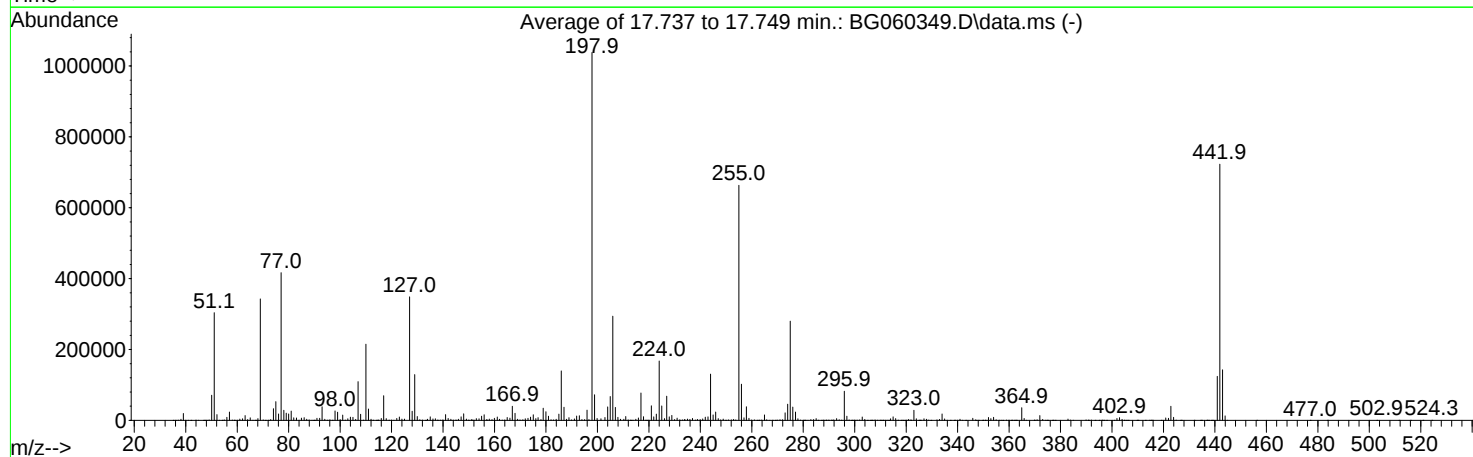


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011824\
Data File : BG060349.D
Acq On : 18 Jan 2024 12:42
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jan 09 04:07:12 2024

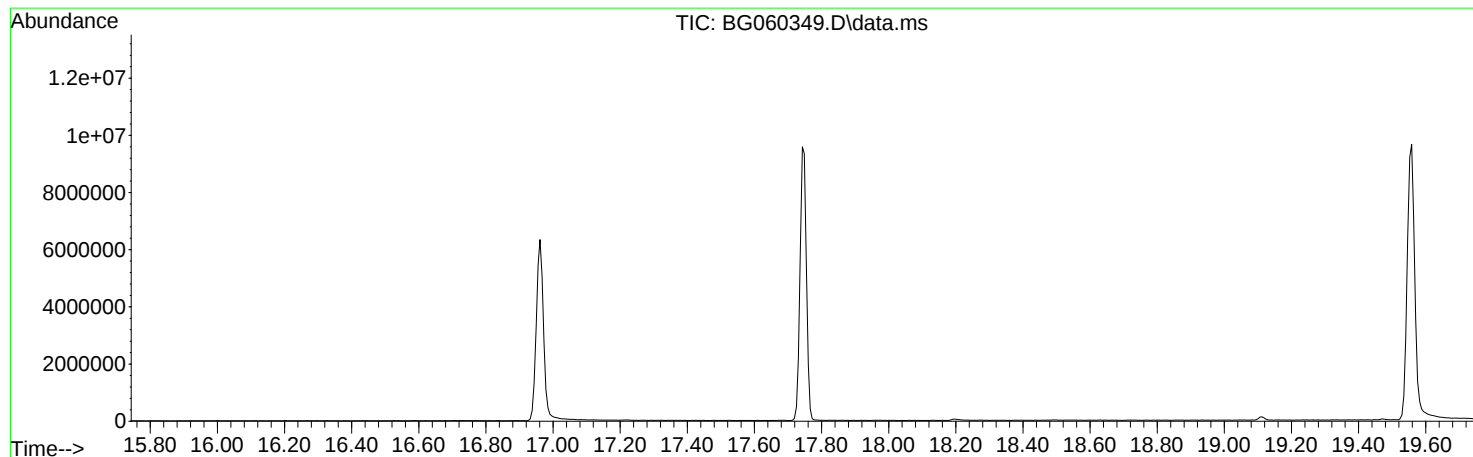




AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2484

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.3	303837	PASS
68	69	0.00	2	1.5	5074	PASS
69	198	0.00	100	33.0	342924	PASS
70	69	0.00	2	0.3	1199	PASS
127	198	10	80	33.6	348587	PASS
197	198	0.00	2	0.2	2401	PASS
198	198	100	100	100.0	1038165	PASS
199	198	5	9	7.0	72317	PASS
275	198	10	60	27.0	280021	PASS
365	198	1	100	3.4	35800	PASS
441	198	0.01	100	11.9	124051	PASS
442	442	50	100	100.0	722965	PASS
443	442	15	24	19.8	142973	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011824\
Data File : BG060349.D
Acq On : 18 Jan 2024 12:42
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 18 13:29:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration

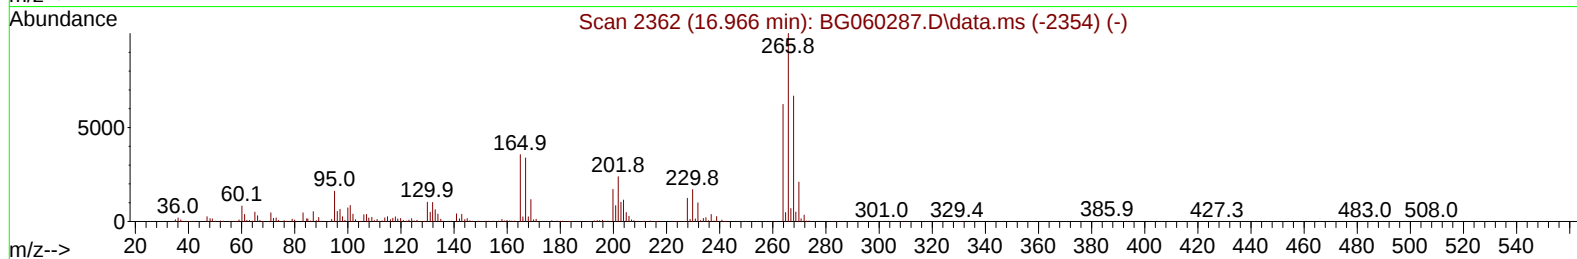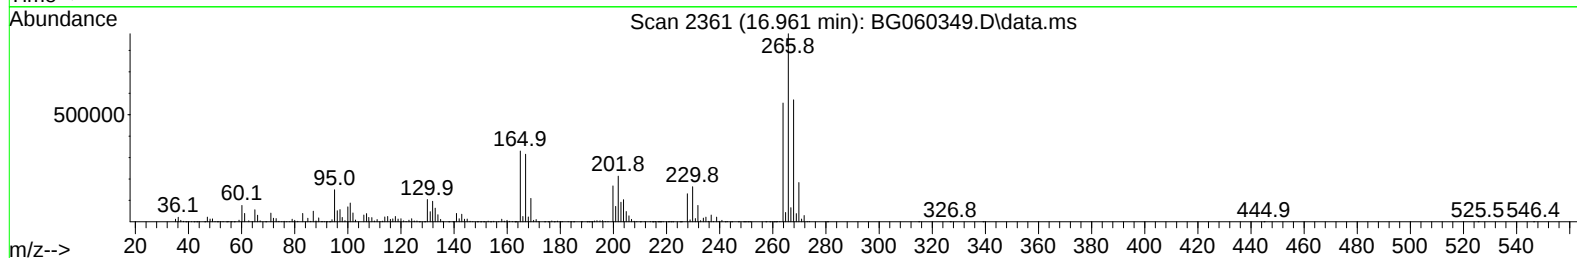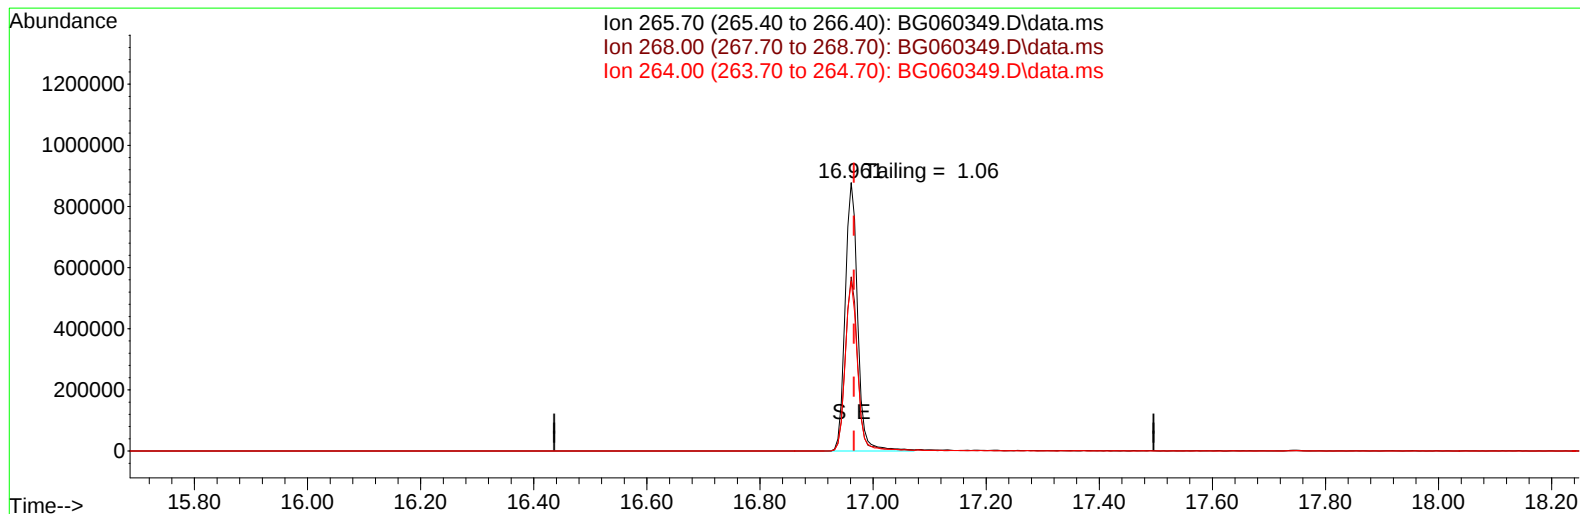

TIC: BG060349.D\data.ms

(70) Pentachlorophenol (C)

16.961min (-0.005) 1425625.23 ng




response 1349301

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	71.80	64.85
264.00	62.30	63.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011824\
Data File : BG060349.D
Acq On : 18 Jan 2024 12:42
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 18 13:29:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration

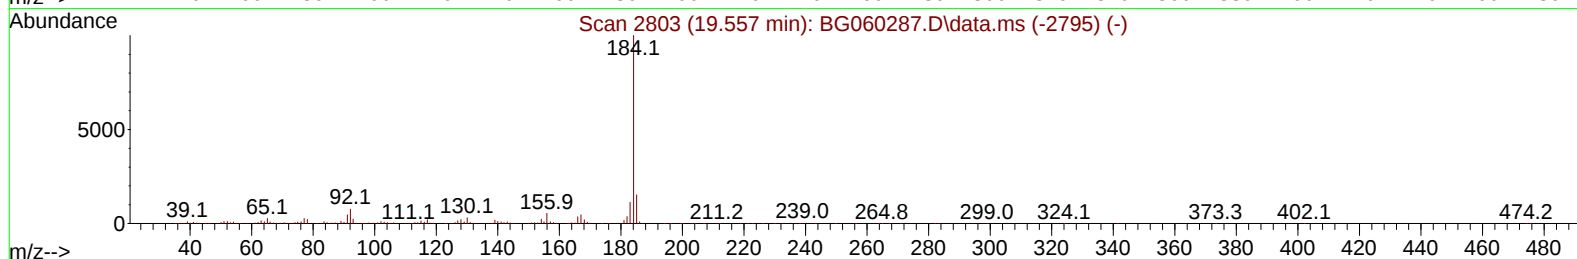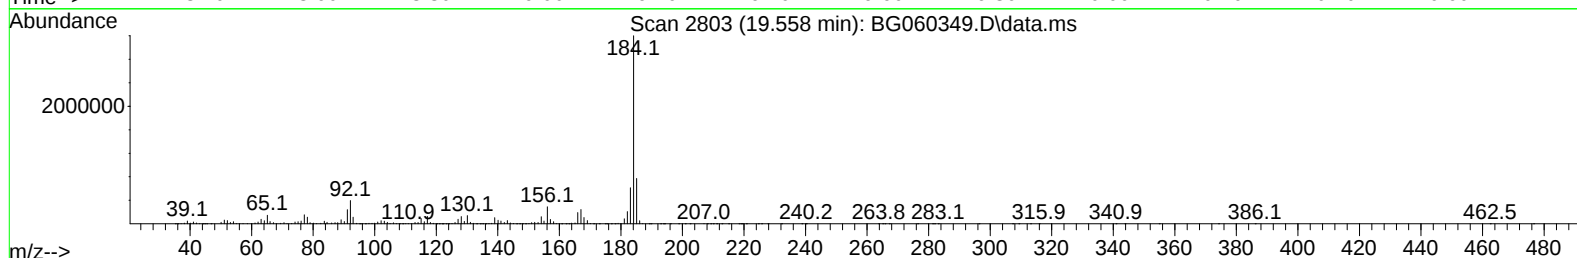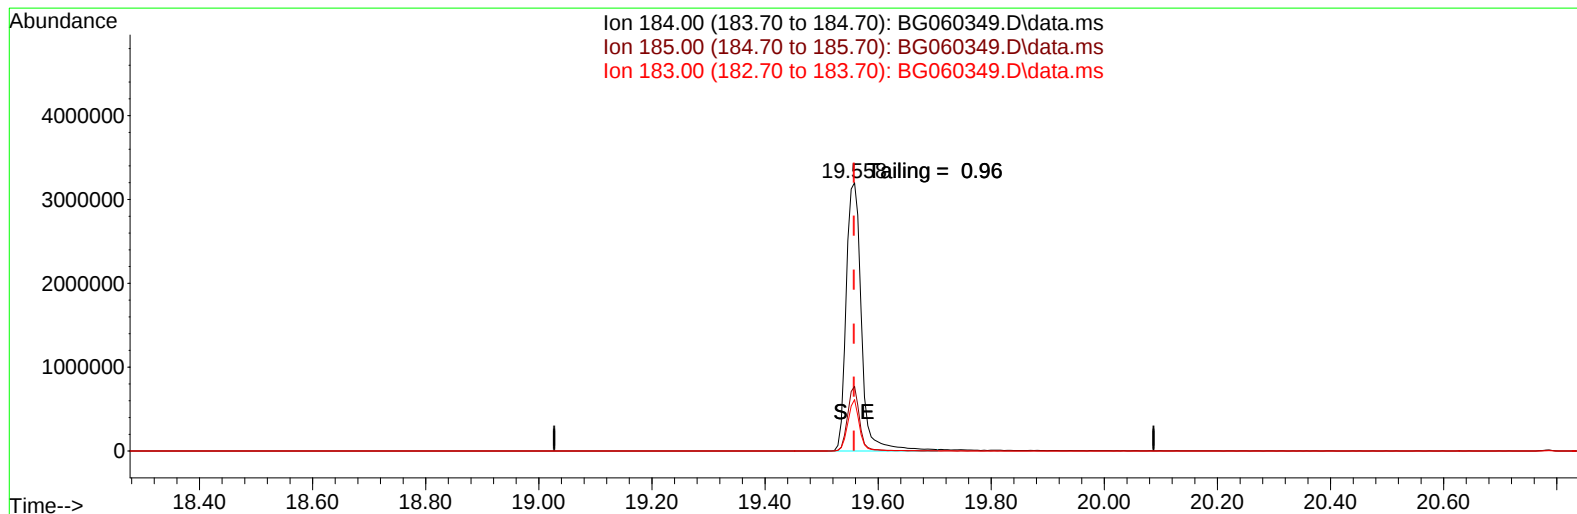

TIC: BG060349.D\data.ms

(77) Benzidine

19.558min (+ 0.001) 4023782.88 ng

response 6031808

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	24.12#
183.00	11.20	19.17#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/18/2024	BNA_G	<u>BG060349.D</u>
Compound Name	Response	Retention Time
DDT	3445869	20.786
DDD	68876	20.398
DDE	2167	19.84
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
71043	3516912	2.02

Instrument :
BNA_G
ClientSampleId :
DFTPP