
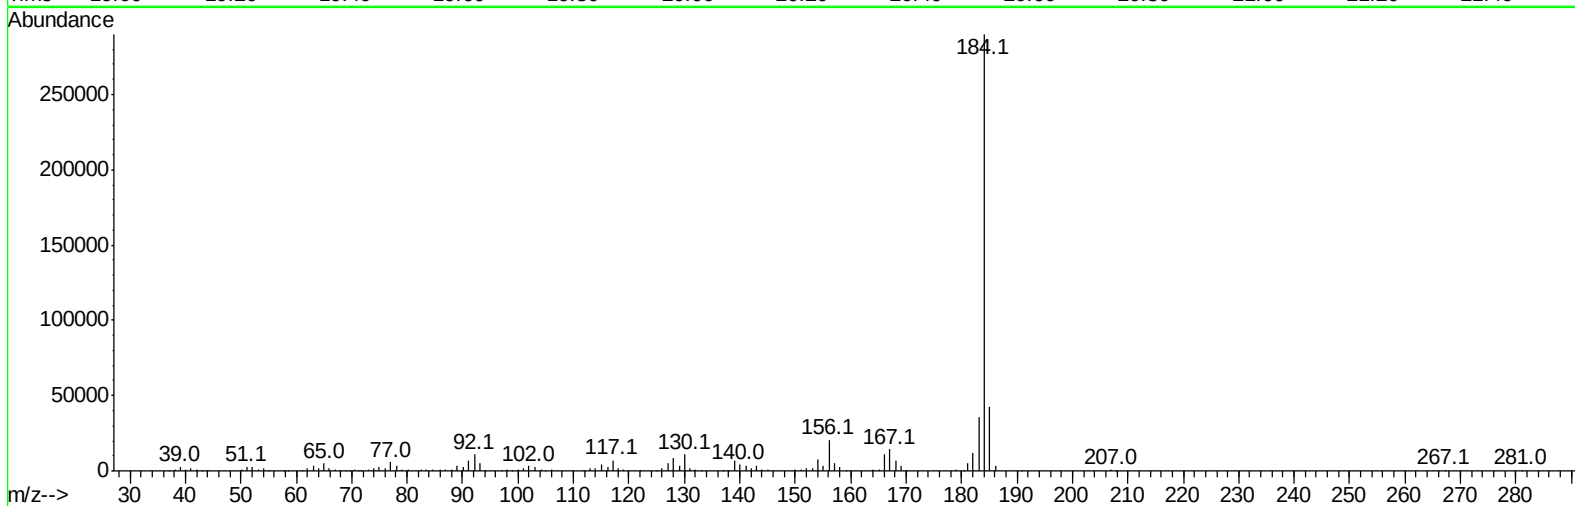


Data Path : U:\HPCHEM1\BNA G\DATA\BG011918\
Data File : BG032150.D
Acq On : 19 Jan 2018 14:05
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 22 00:35:23 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG011218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 18 10:13:16 2018
Response via : Initial Calibration

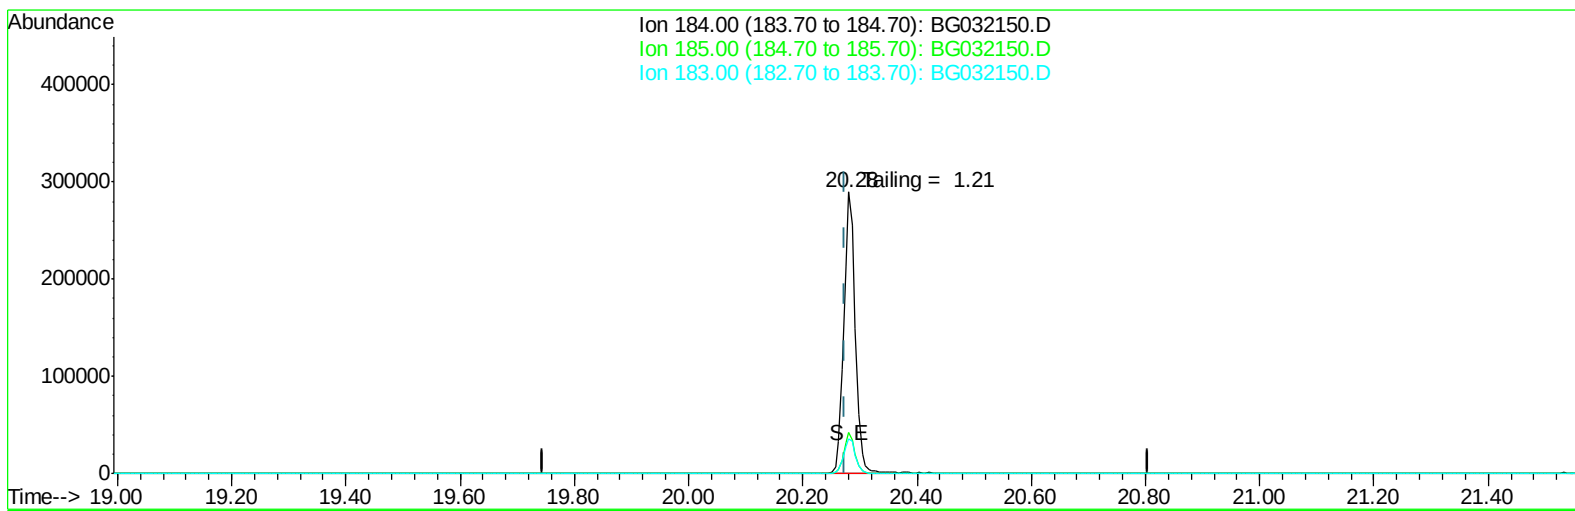

TIC: BG032150.D

(76) Benzidine



20.280min (+0.005) 240192.92ng

response 408429

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.66
183.00	13.30	12.44
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA G\DATA\BG011918\
Data File : BG032150.D
Acq On : 19 Jan 2018 14:05
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 22 00:35:23 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG011218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 18 10:13:16 2018
Response via : Initial Calibration

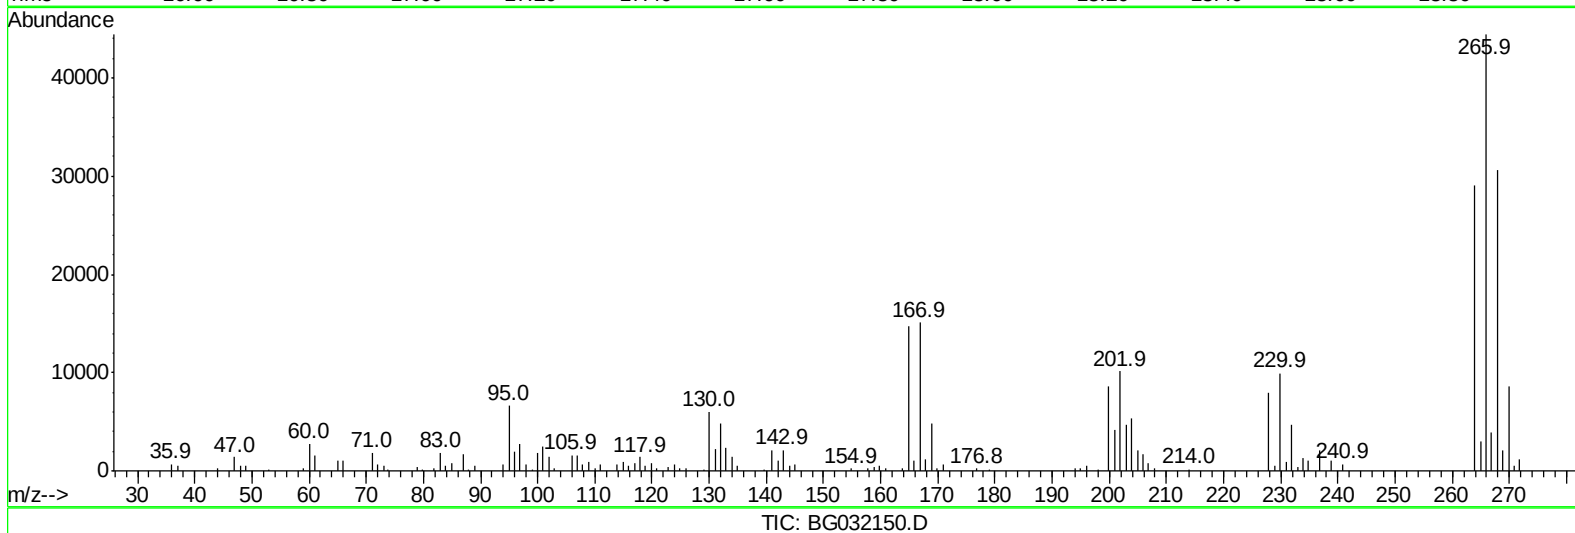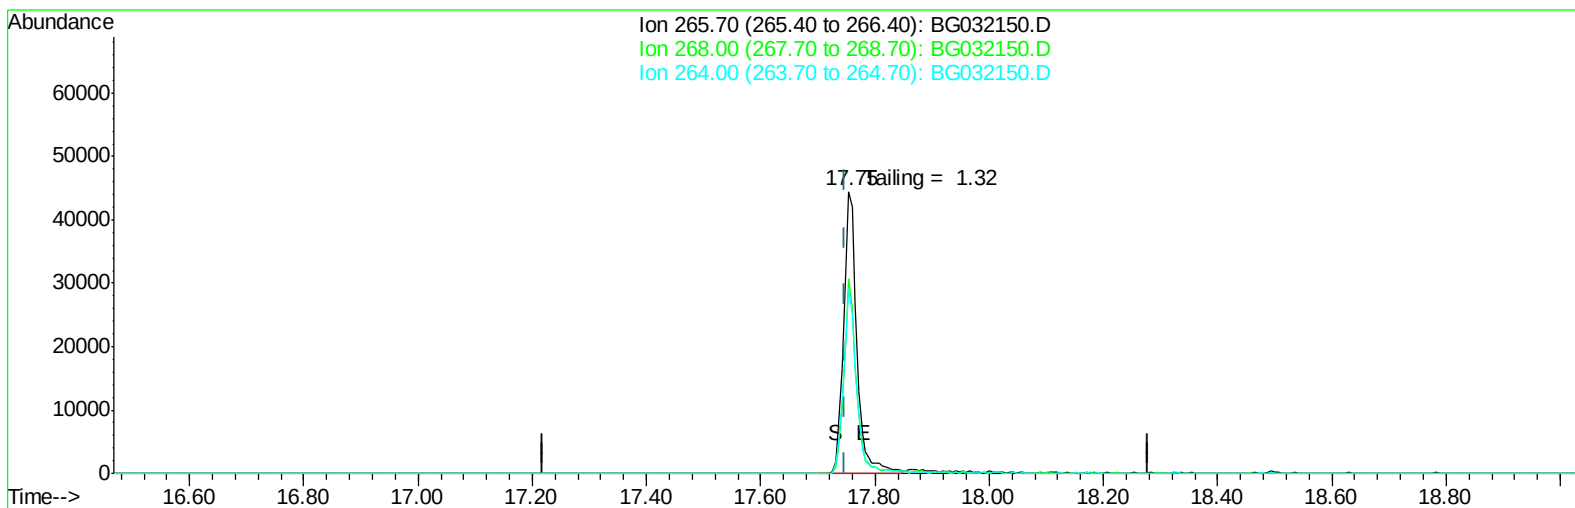

TIC: BG032150.D

(69) Pentachlorophenol (C)

17.754min (+0.005) 18515.20ng

response 73213

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	69.05
264.00	62.00	65.45
0.00	0.00	0.00