
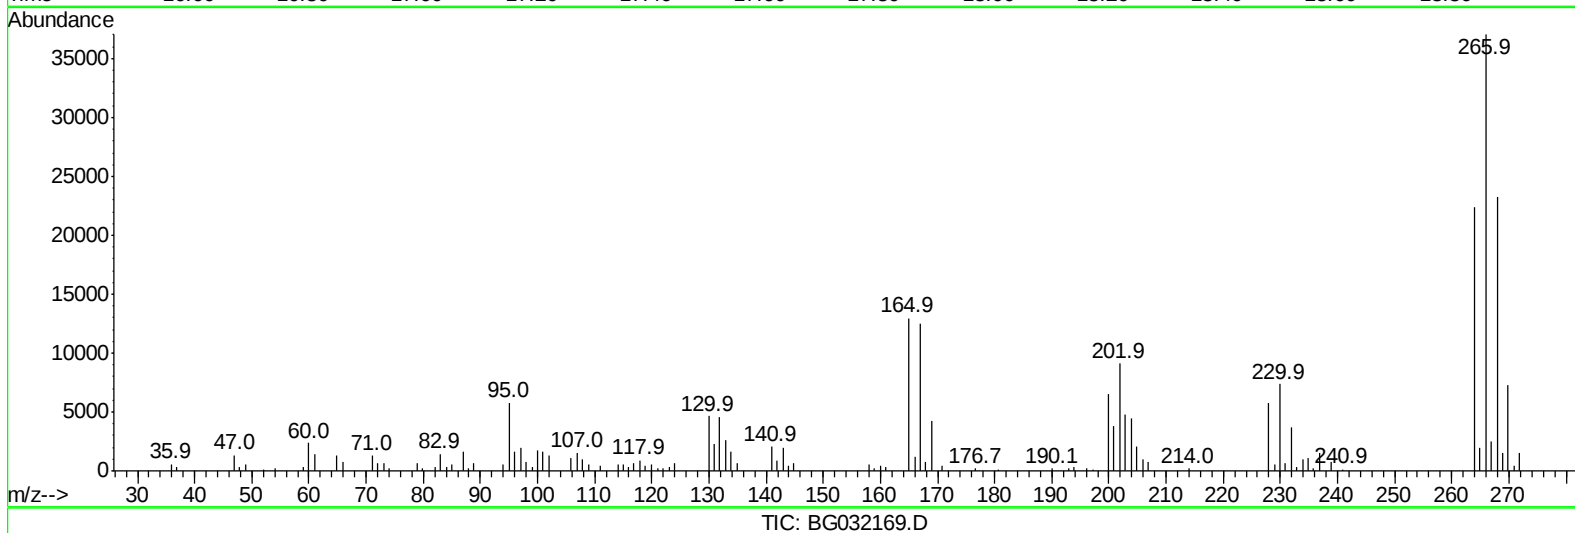


Data Path : U:\HPCHEM1\BNA G\DATA\BG011918\
Data File : BG032169.D
Acq On : 20 Jan 2018 3:37
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 22 00:36:53 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG011218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 18 10:13:16 2018
Response via : Initial Calibration

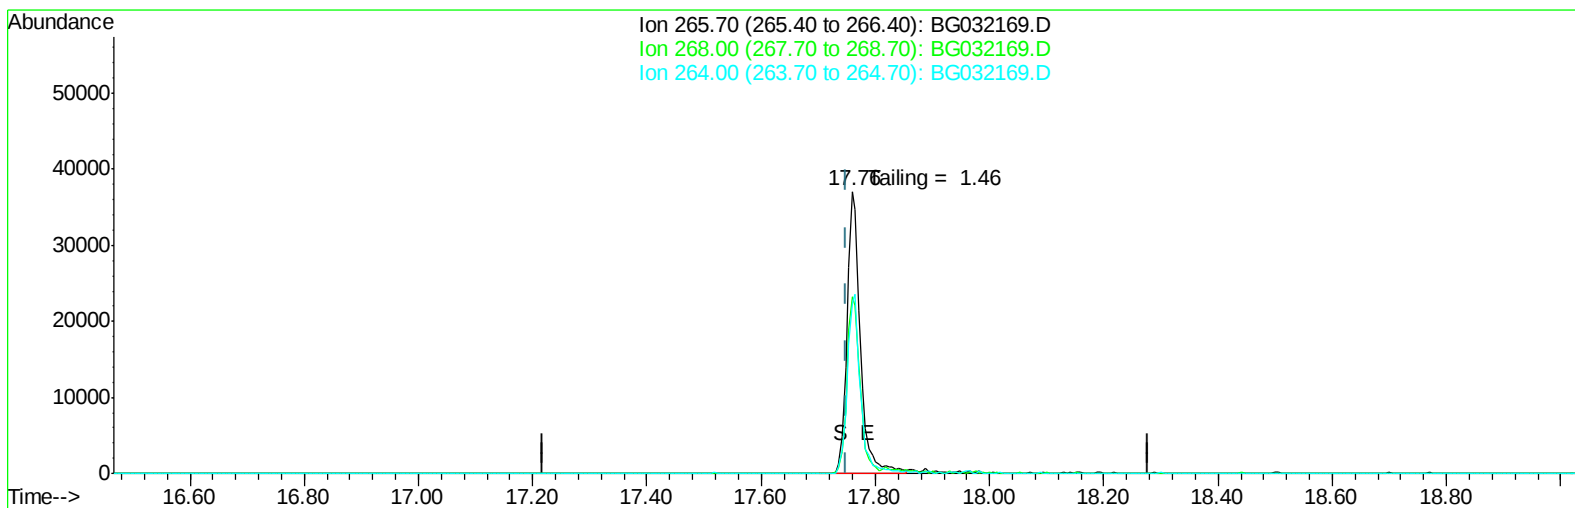

(69) Pentachlorophenol (C)



17.759min (+0.010) 13603.27ng

response 60360

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.86
264.00	62.00	60.40
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA G\DATA\BG011918\
Data File : BG032169.D
Acq On : 20 Jan 2018 3:37
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 22 00:36:53 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG011218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 18 10:13:16 2018
Response via : Initial Calibration

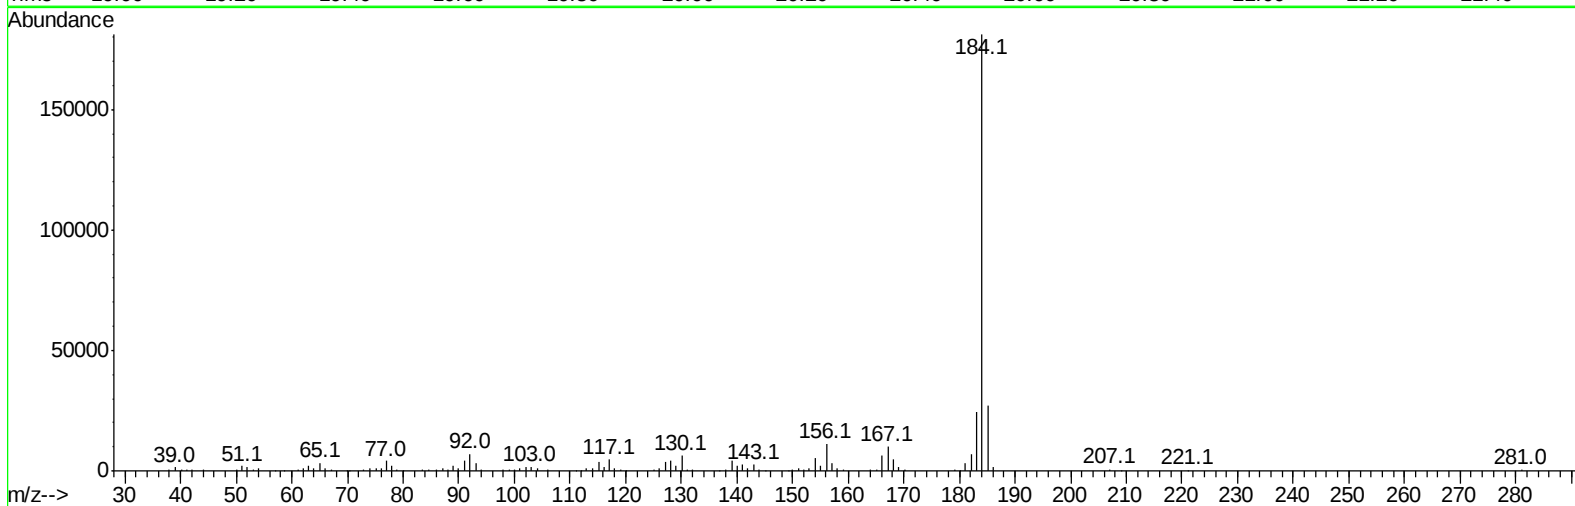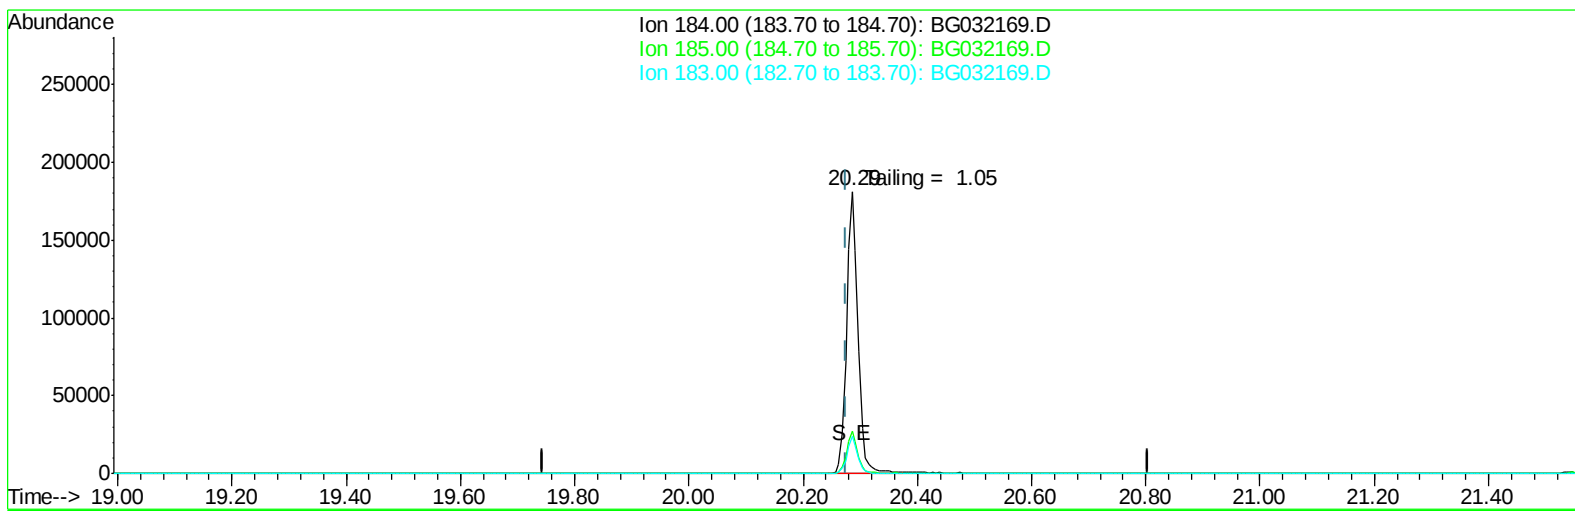

TIC: BG032169.D

(76) Benzidine

20.286min (+0.010) 0.00ng

response 251015

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.95
183.00	13.30	13.41
0.00	0.00	0.00