

Data Path : Z:\HPCHEM1\BNA G\DATA\BG011918\
 Data File : BG032153.D
 Acq On : 19 Jan 2018 15:58
 Operator : SJ/JU
 Sample : PB105755BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB105755BL

Quant Time: Jan 19 23:46:50 2018
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG011218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 18 10:13:16 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.74	152	38329	20.00	ng	0.00
21) Naphthalene-d8	11.62	136	154260	20.00	ng	0.00
38) Acenaphthene-d10	15.38	164	109538	20.00	ng	0.00
63) Phenanthrene-d10	18.11	188	316696	20.00	ng	0.00
75) Chrysene-d12	22.44	240	444401	20.00	ng	0.00
86) Perylene-d12	26.15	264	453773	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	6.17	112	271906	129.74	ng	0.00
7) Phenol-d6	7.85	99	338045	128.08	ng	0.00
23) Nitrobenzene-d5	9.94	82	197770	86.74	ng	0.00
41) 2,4,6-Tribromophenol	16.86	330	238063	131.34	ng	0.00
44) 2-Fluorobiphenyl	14.01	172	720932	81.61	ng	0.00
78) Terphenyl-d14	20.65	244	1650199	81.99	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG011918\
Data File : BG032153.D
Acq On : 19 Jan 2018 15:58
Operator : SJ/JU
Sample : PB105755BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB105755BL

Quant Time: Jan 19 23:46:50 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG011218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 18 10:13:16 2018
Response via : Initial Calibration

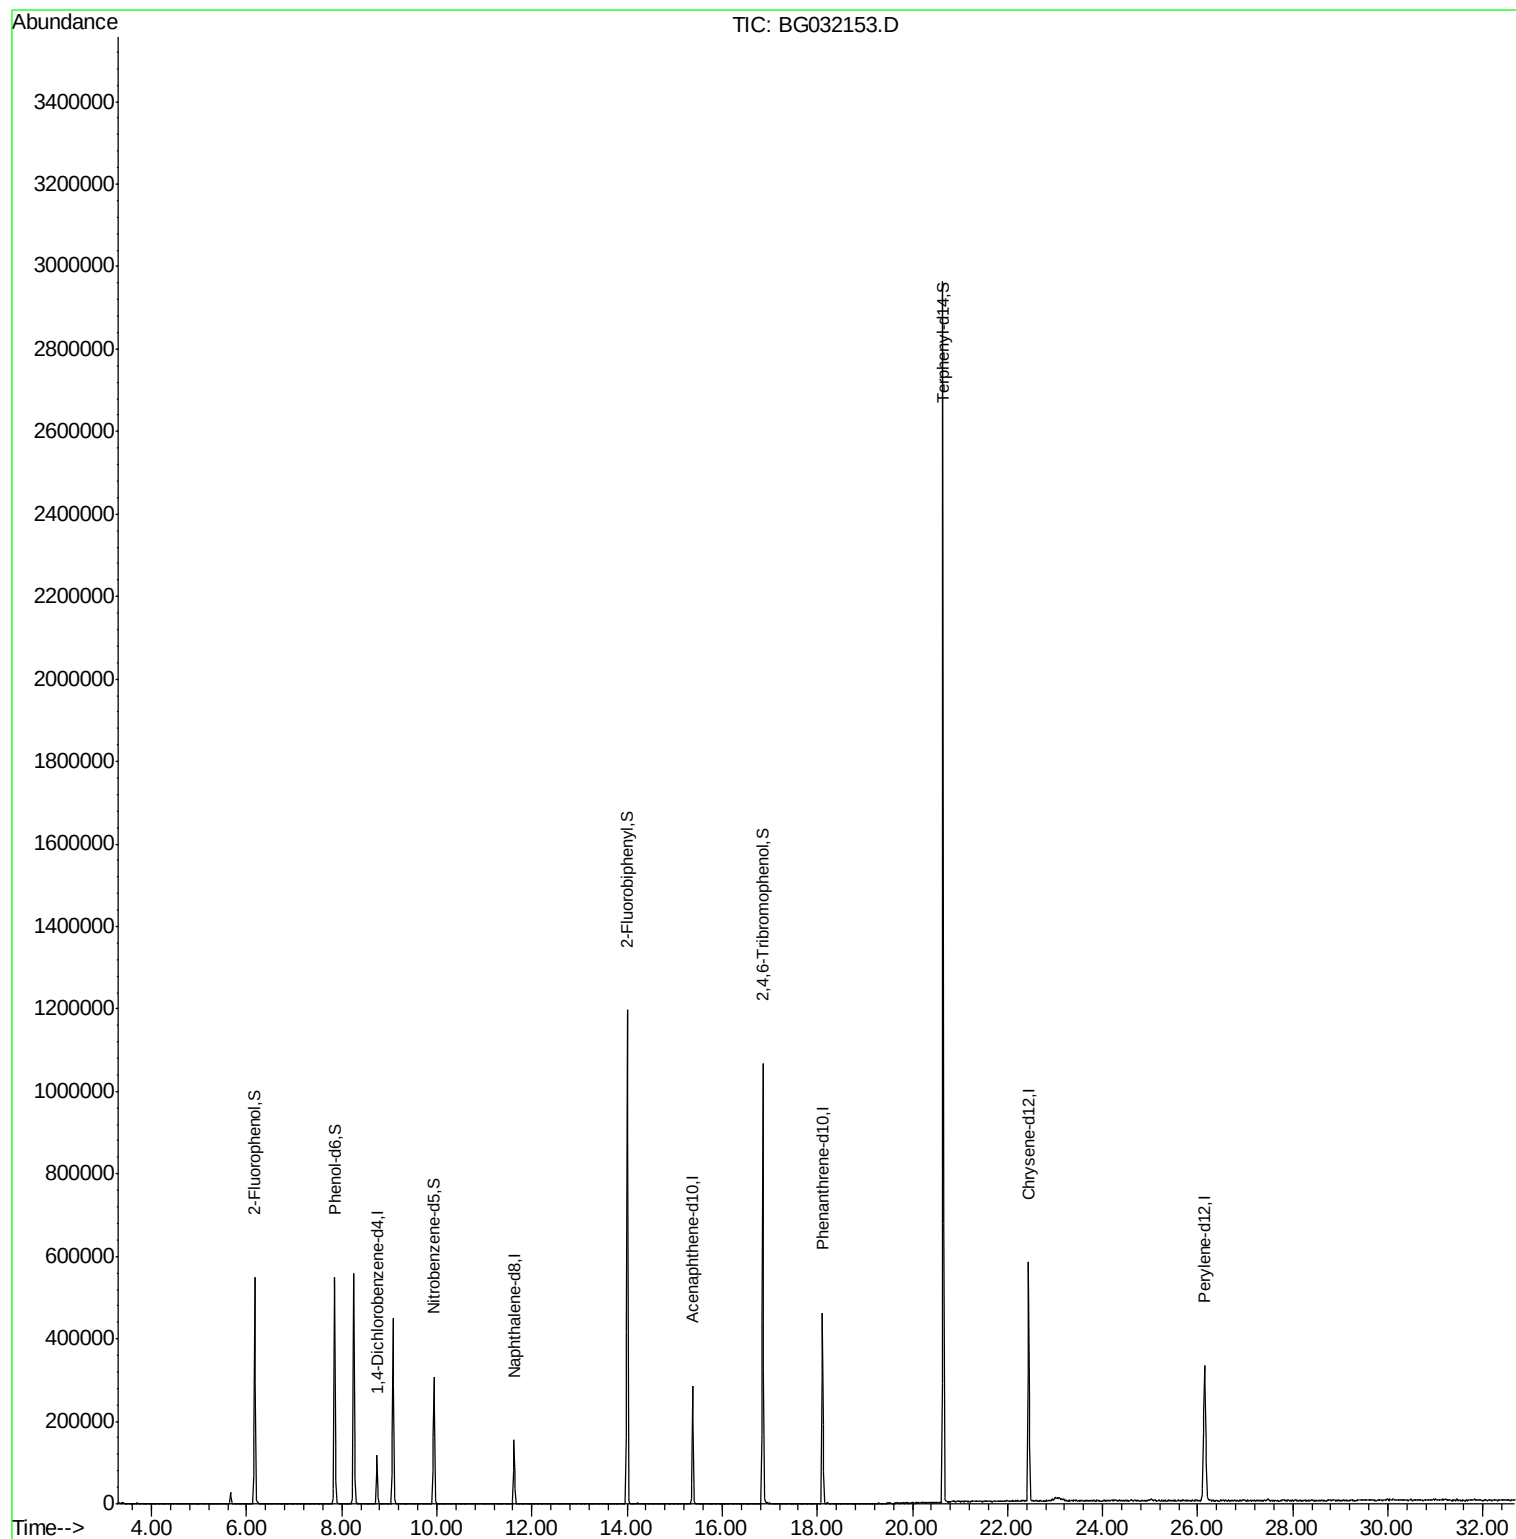




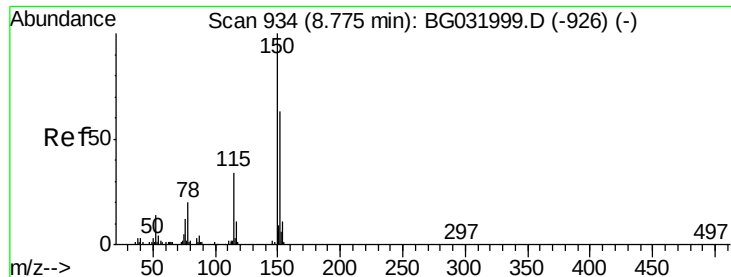


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.74 min Scan# 928
Delta R.T. 0.00 min
Lab File: BG032153.D
Acq: 19 Jan 2018 15:58

Instrument :
BNA_G
ClientSampleId :
PB105755BL




Tot Ion:152 Resp: 38329
Ion Ratio Lower Upper
152 100
150 147.3 126.6 189.8
115 50.8 53.0 79.4#

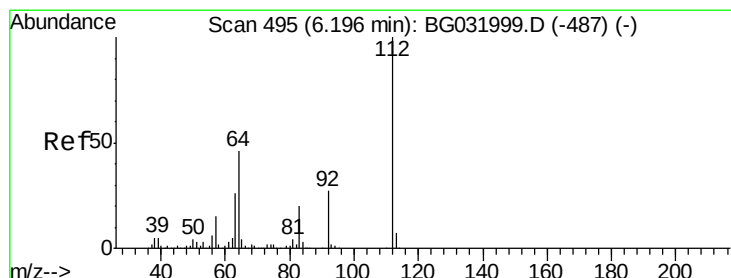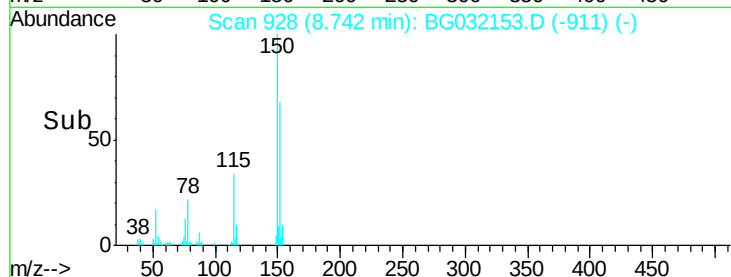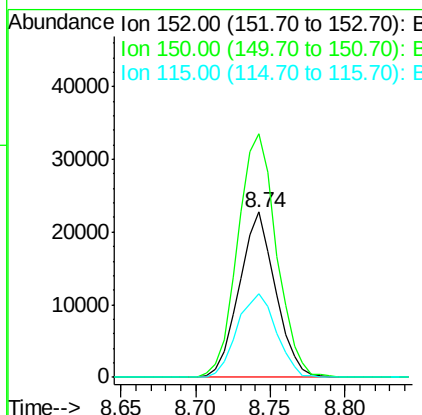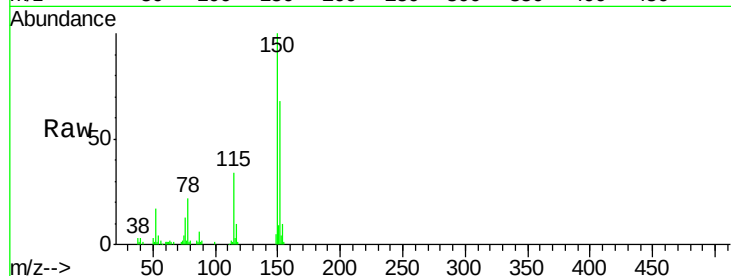


#5

2-Fluorophenol
Concen: 129.745 ng
RT: 6.17 min Scan# 490
Delta R.T. 0.00 min
Lab File: BG032153.D
Acq: 19 Jan 2018 15:58

Tgt Ion:112 Resp: 271906
Ion Ratio Lower Upper
112 100
64 51.9 56.3 84.5#
63 30.7 30.1 45.1

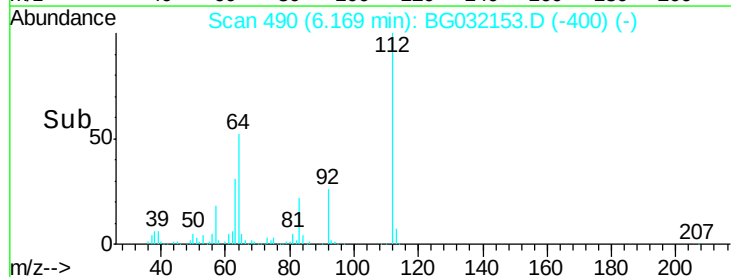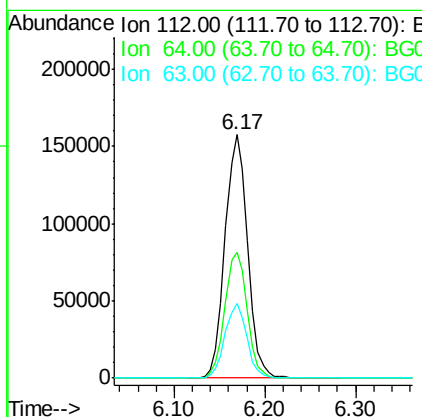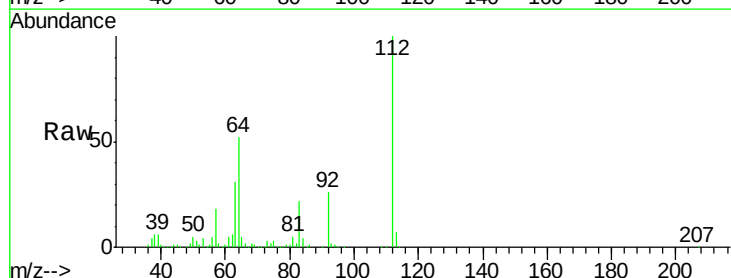

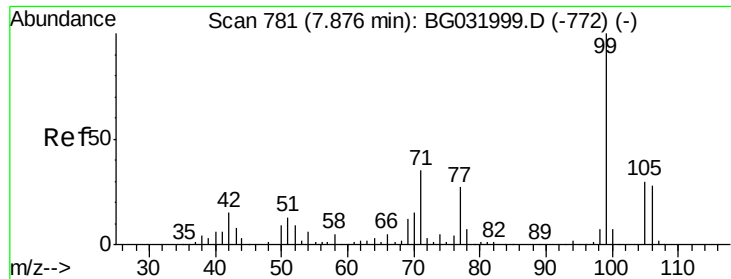

#7

Phenol-d6

Concen: 128.076 ng

RT: 7.85 min Scan# 776

Delta R.T. 0.00 min

Lab File: BG032153.D

Acq: 19 Jan 2018 15:58

Instrument :

BNA_G

ClientSampleId :

PB105755BL


Tot Ion: 99 Resp: 338045

Ion Ratio Lower Upper




99 100

42 15.9 14.1 21.1

71 42.7 26.1 39.1#

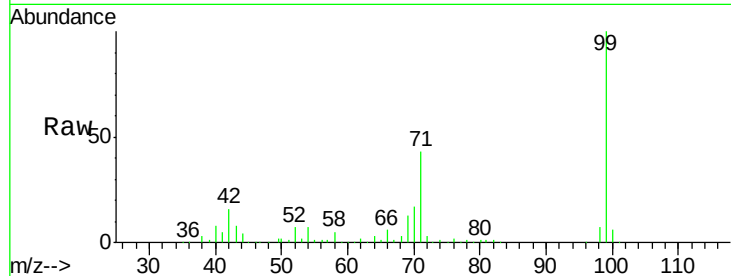

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

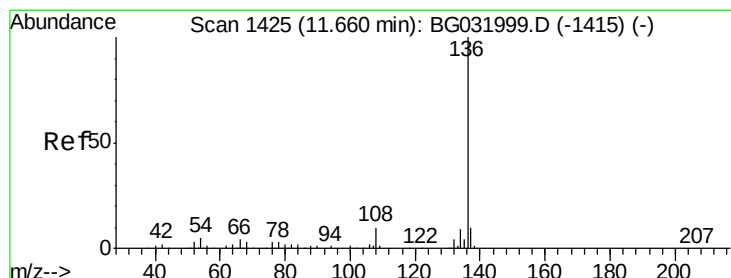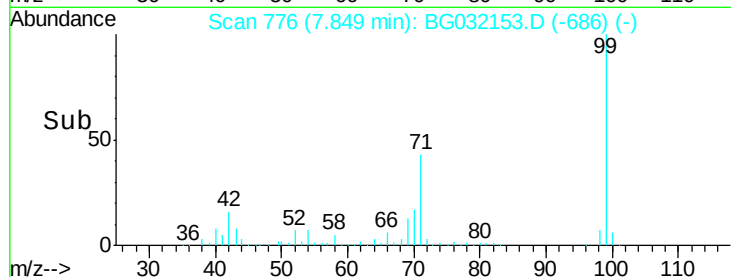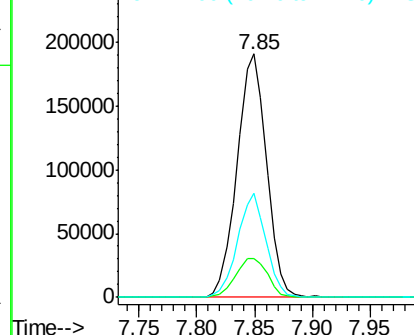

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 11.62 min Scan# 1418

Delta R.T. -0.01 min

Lab File: BG032153.D

Acq: 19 Jan 2018 15:58

Tgt Ion: 136 Resp: 154260


Ion Ratio Lower Upper

136 100



137 11.5 9.2 13.8


54 4.9 10.3 15.5#

68 3.6 4.5 6.7#

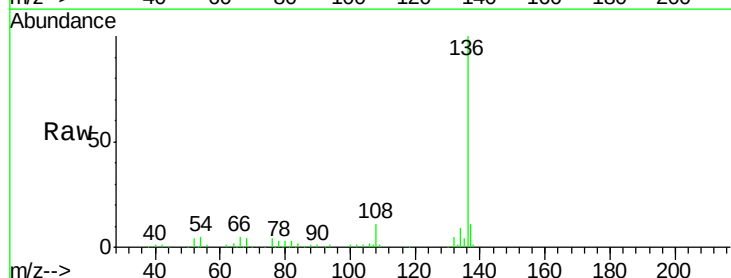

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



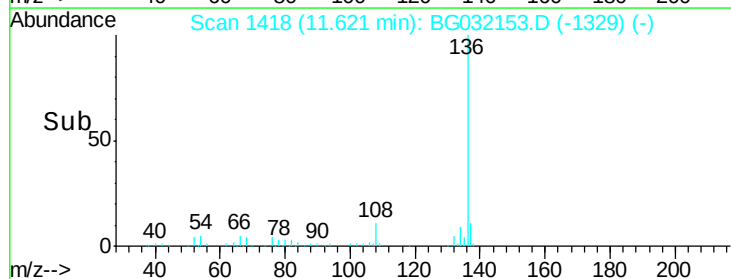
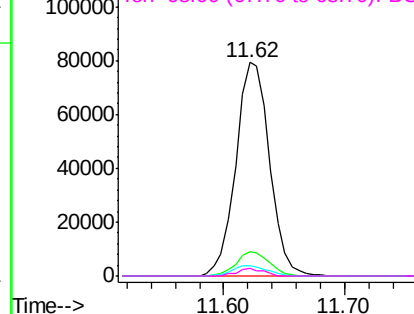


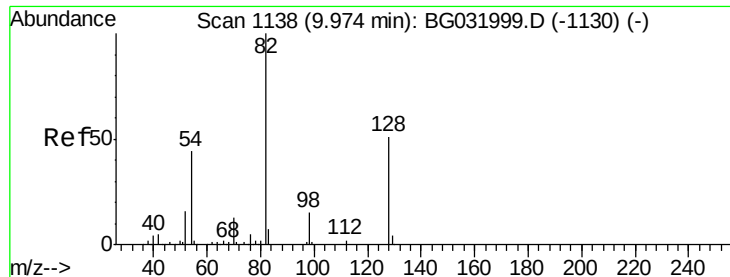

#23
 Nitrobenzene-d5
 Concen: 86.737 ng
 RT: 9.94 min Scan# 1132
 Delta R.T. 0.00 min
 Lab File: BG032153.D
 Acq: 19 Jan 2018 15:58




Instrument :
 BNA_G
 ClientSampleId :
 PB105755BL


Tot Ion: 82 Resp: 197770
 Ion Ratio Lower Upper
 82 100
 128 47.1 29.7 44.5#
 54 46.6 43.1 64.7

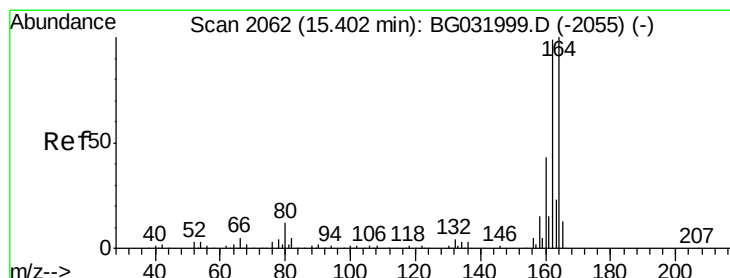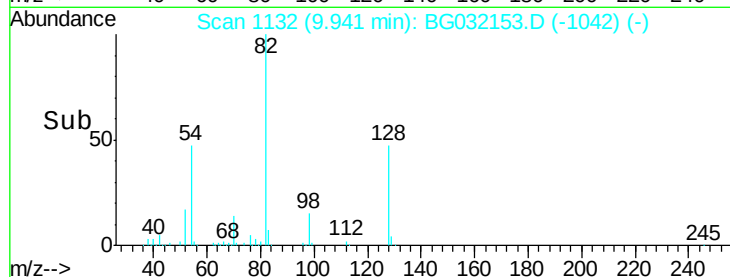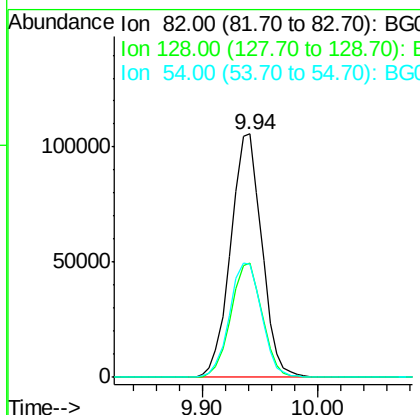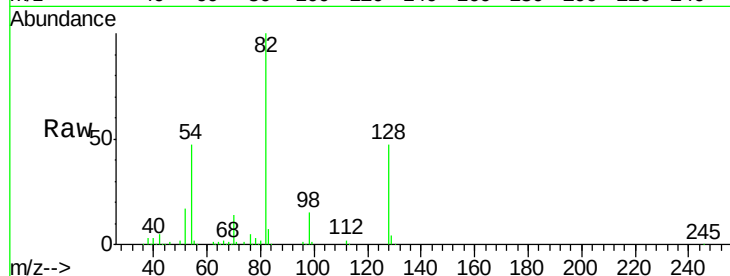

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 15.38 min Scan# 2057
 Delta R.T. -0.01 min
 Lab File: BG032153.D
 Acq: 19 Jan 2018 15:58

Tgt Ion: 164 Resp: 109538
 Ion Ratio Lower Upper
 164 100
 162 101.3 78.8 118.2
 160 41.5 35.4 53.0

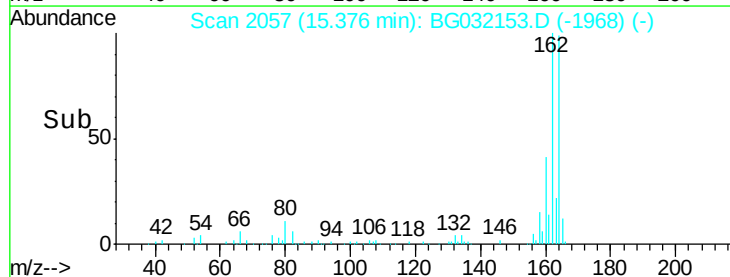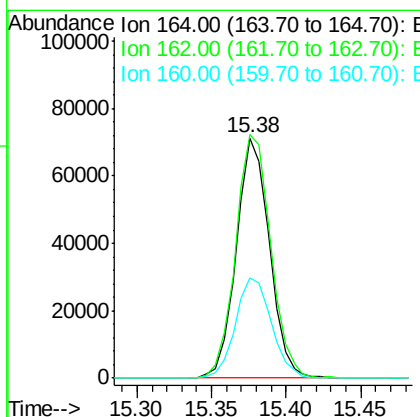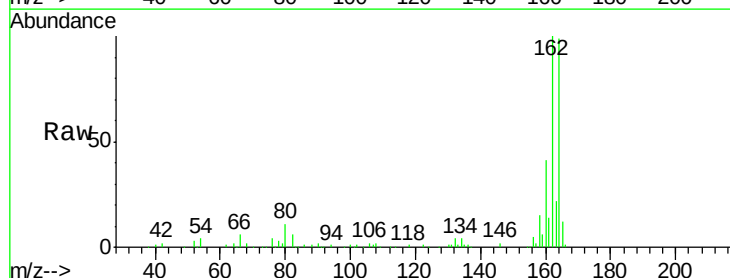


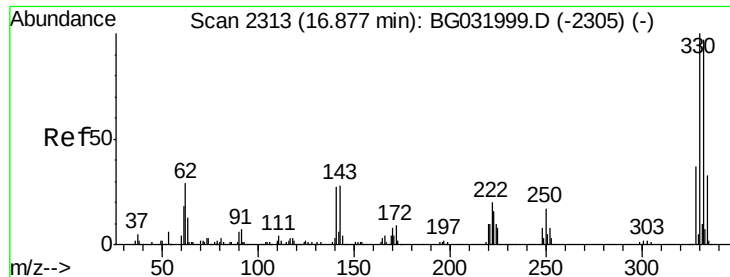

#41
 2,4,6-Tribromophenol
 Concen: 131.338 ng
 RT: 16.86 min Scan# 2309
 Delta R.T. 0.00 min
 Lab File: BG032153.D
 Acq: 19 Jan 2018 15:58

Instrument :
 BNA_G
 ClientSampleId :
 PB105755BL

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.7	77.0	115.6
141	29.2	25.2	37.8



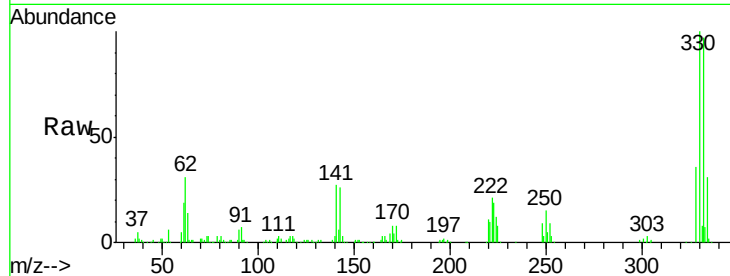


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

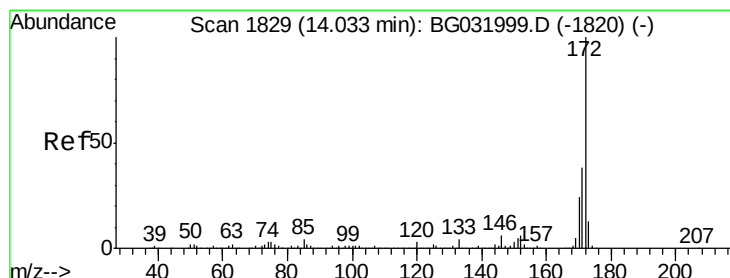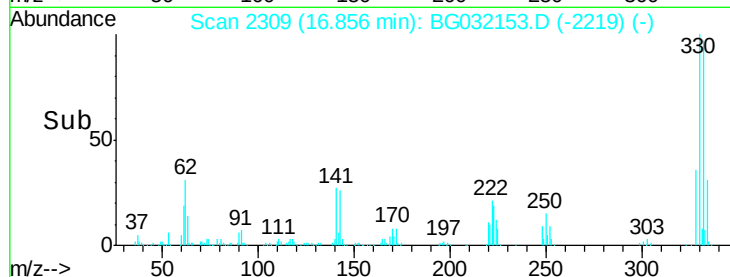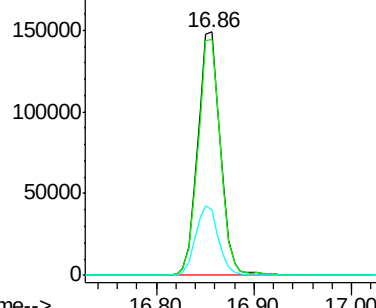

#44
 2-Fluorobiphenyl
 Concen: 81.608 ng
 RT: 14.01 min Scan# 1824
 Delta R.T. 0.00 min
 Lab File: BG032153.D
 Acq: 19 Jan 2018 15:58

Tgt Ion	Ratio	Lower	Upper
172	100		
171	37.7	30.0	45.0
170	23.1	19.5	29.3


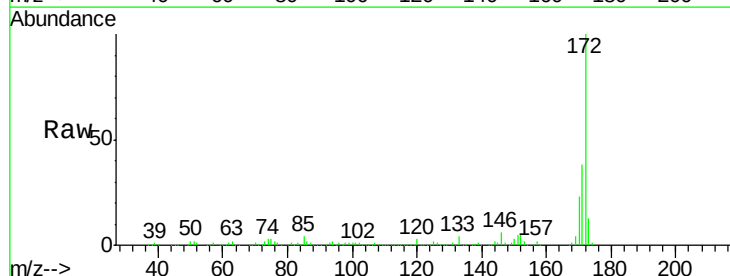



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

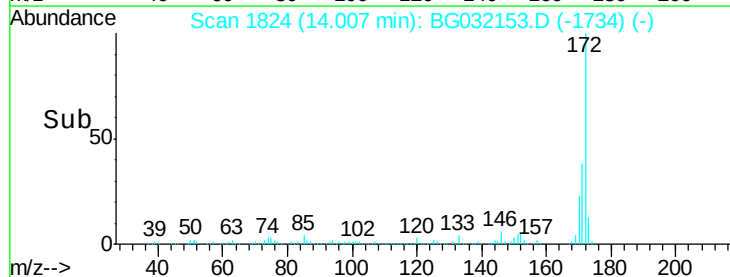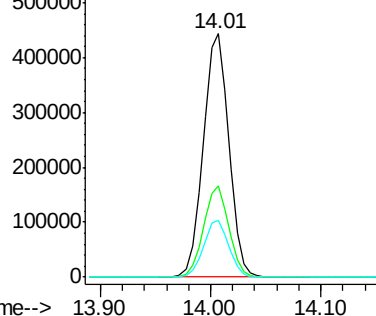


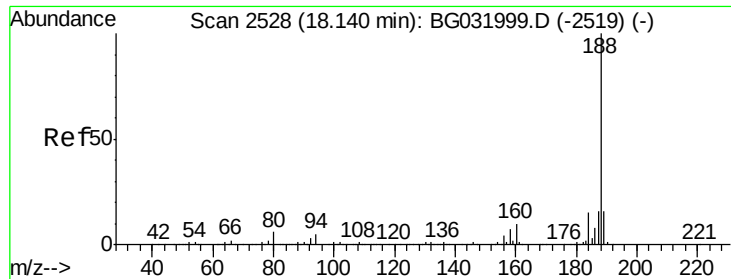




#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 18.11 min Scan# 2522
Delta R.T. -0.01 min
Lab File: BG032153.D
Acq: 19 Jan 2018 15:58

Instrument :
BNA_G
ClientSampleId :
PB105755BL

Tot Ion:188 Resp: 316696
Ion Ratio Lower Upper
188 100
94 4.1 6.9 10.3#
80 4.7 7.7 11.5#

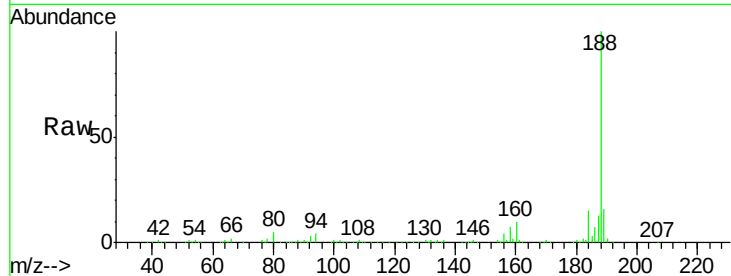


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BGC
Ion 80.00 (79.70 to 80.70): BGC

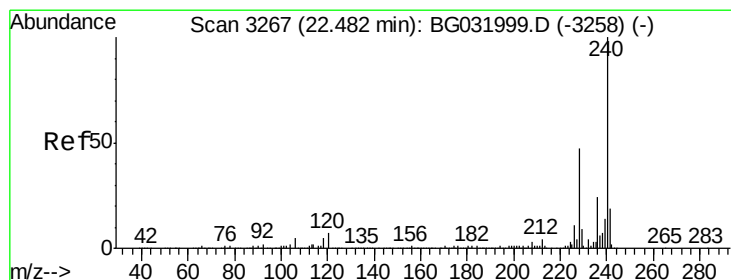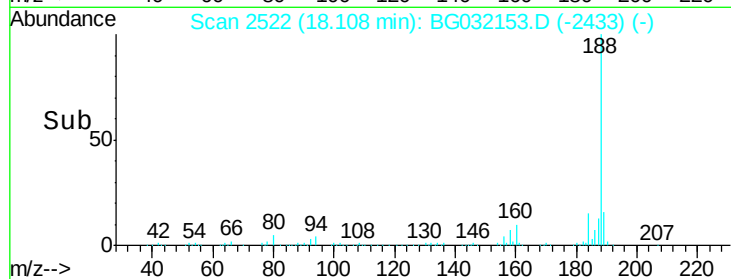
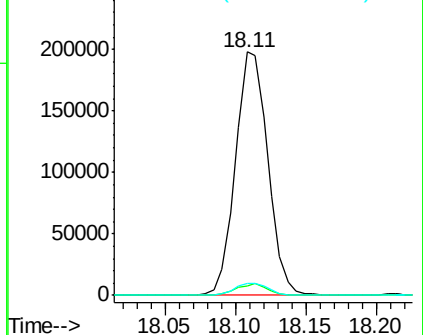



#75
Chrysene-d12
Concen: 20.000 ng
RT: 22.44 min Scan# 3260
Delta R.T. -0.01 min
Lab File: BG032153.D
Acq: 19 Jan 2018 15:58

Tgt Ion:240 Resp: 444401
Ion Ratio Lower Upper
240 100
120 5.2 6.8 10.2#
236 25.5 20.9 31.3

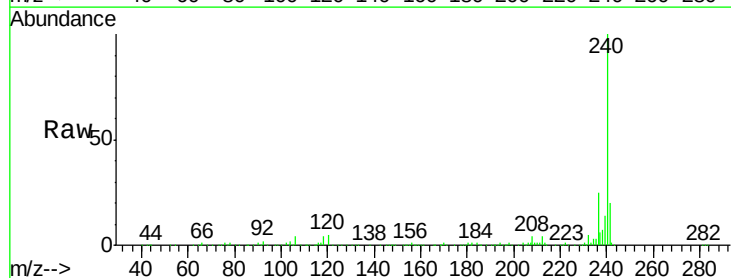

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

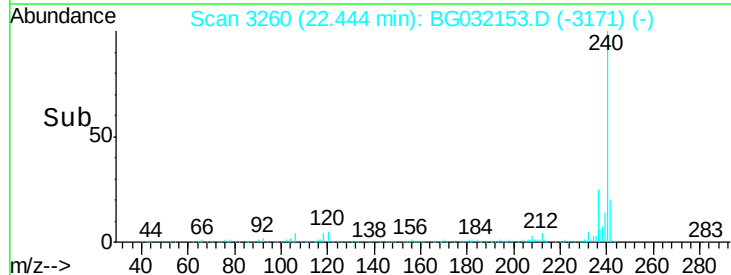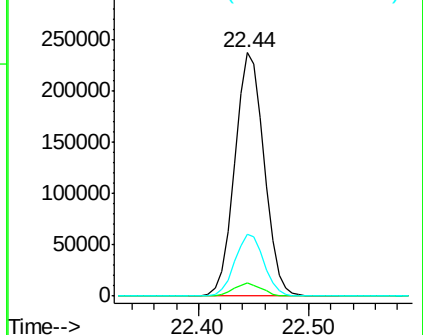

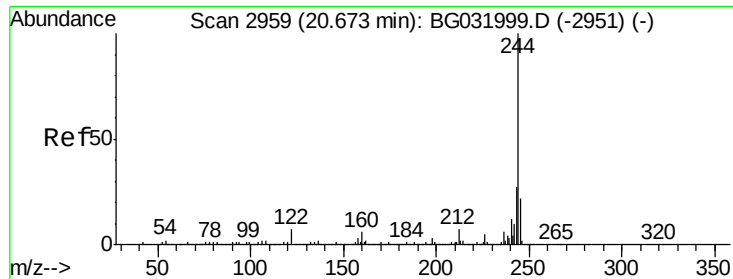

#78

Terphenyl-d14

Concen: 81.992 ng

RT: 20.65 min Scan# 2954

Delta R.T. -0.01 min

Lab File: BG032153.D

Acq: 19 Jan 2018 15:58

Instrument :

BNA_G

ClientSampleId :

PB105755BL


Tot Ion:244 Resp: 1650199

Ion Ratio Lower Upper

244 100

212 7.9 5.8 8.8




122 6.6 7.0 10.4#

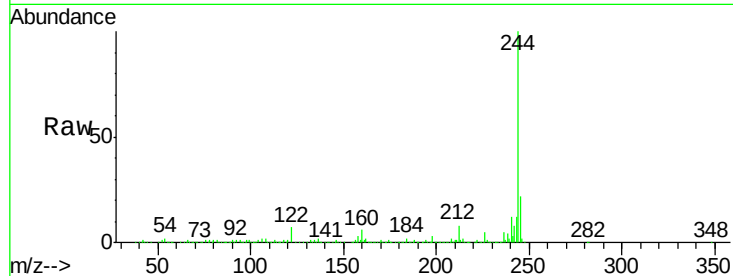

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

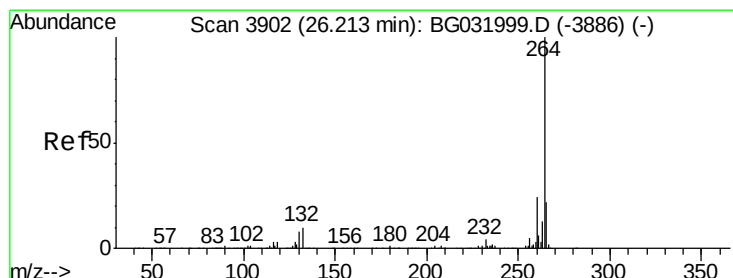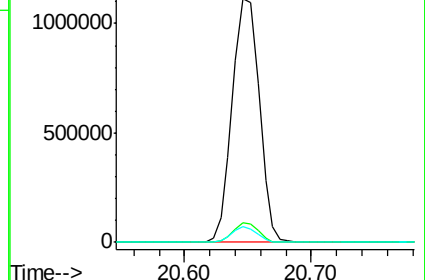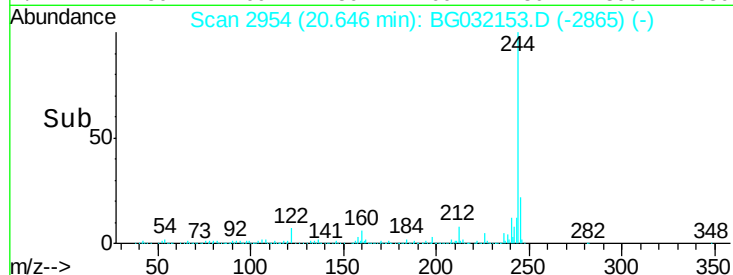

#86

Perylene-d12

Concen: 20.000 ng

RT: 26.15 min Scan# 3890

Delta R.T. -0.01 min

Lab File: BG032153.D

Acq: 19 Jan 2018 15:58


Tgt Ion:264 Resp: 453773

Ion Ratio Lower Upper

264 100

260 23.1 17.4 26.0

265 21.6 17.7 26.5

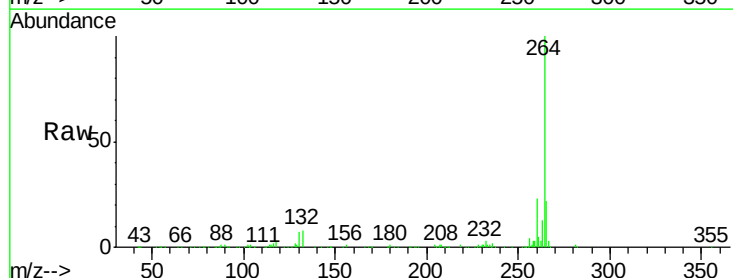

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

