


Data Path : Z:\HPCHEM1\BNA G\Data\BG011918\
 Data File : BG032150.D
 Acq On : 19 Jan 2018 14:05
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG011218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 18 10:13:16 2018

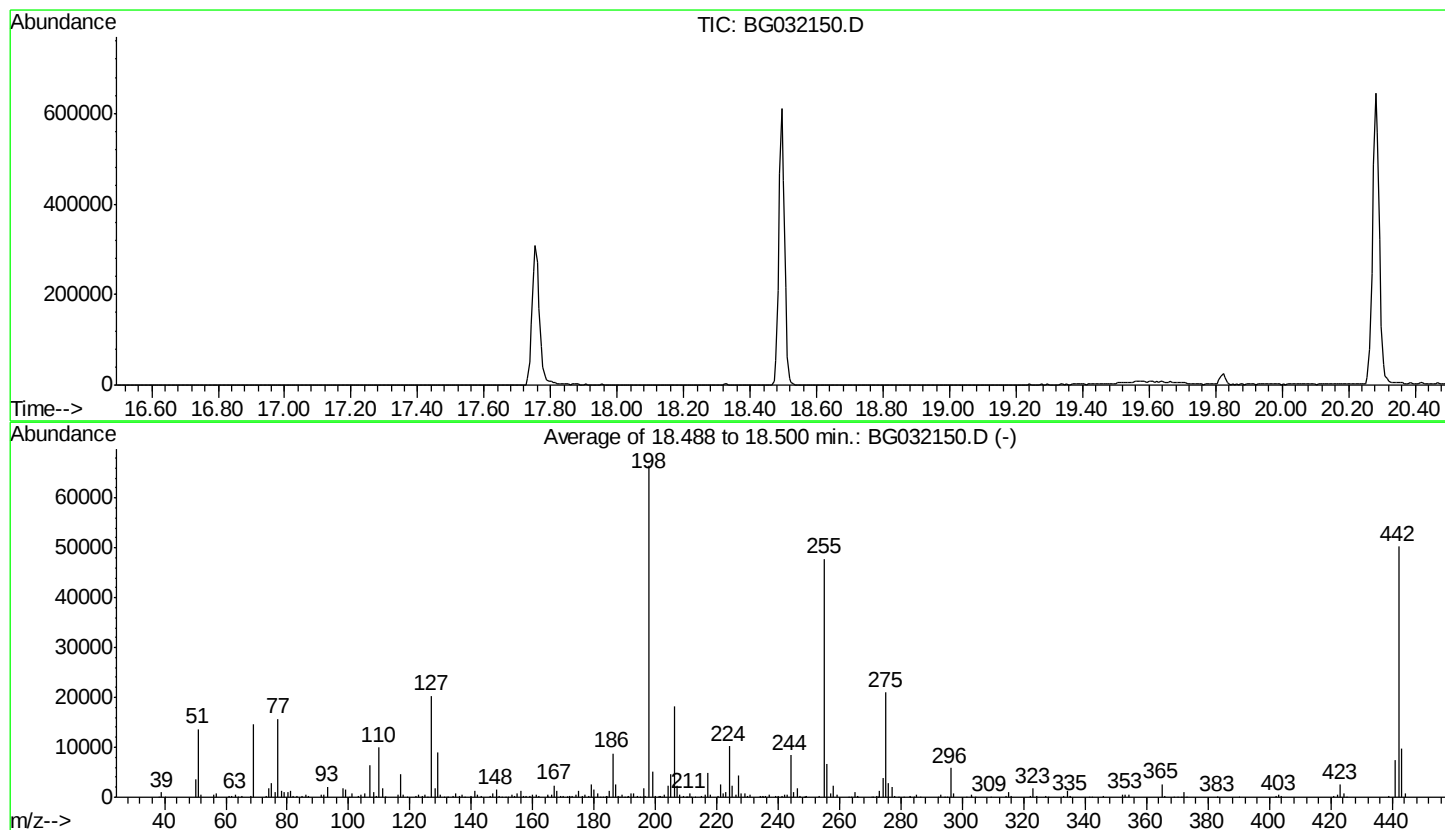

AutoFind: Scans 2587, 2588, 2589; Background Corrected with Scan 2581

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	20.5	13611	PASS
68	69	0.00	2	1.7	254	PASS
69	198	0.00	100	22.1	14698	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	30.6	20314	PASS
197	198	0.00	2	0.2	164	PASS
198	198	100	100	100.0	66461	PASS
199	198	5	9	7.6	5024	PASS
275	198	10	60	31.6	20981	PASS
365	198	1	100	3.9	2602	PASS
441	442	0.01	24	15.0	7518	PASS
442	198	50	100	75.5	50205	PASS
443	442	15	24	19.5	9814	PASS