


Data Path : Z:\HPCHEM1\BNA G\Data\BG011918\
 Data File : BG032169.D
 Acq On : 20 Jan 2018 3:37
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG011218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 18 10:13:16 2018

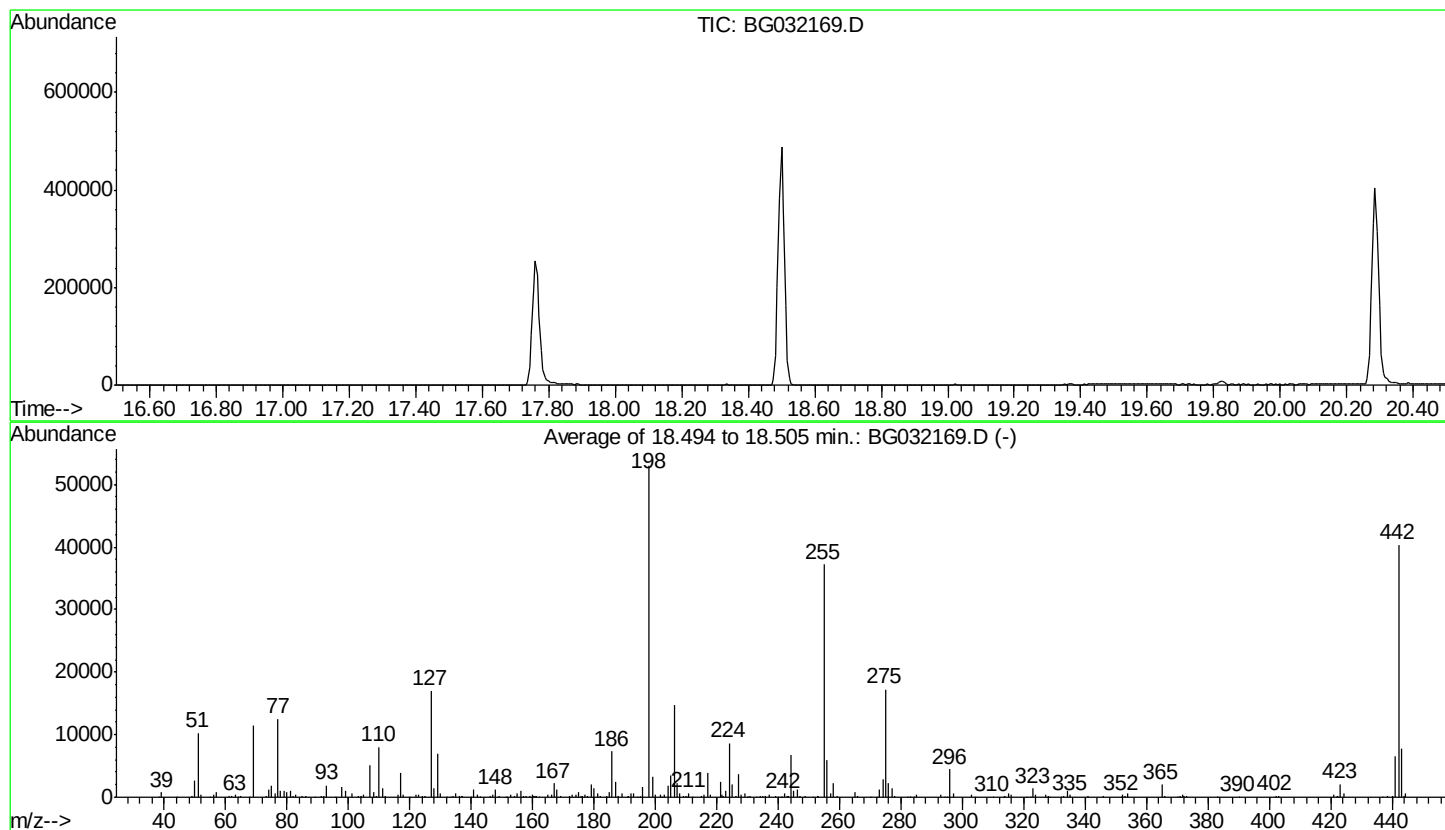

AutoFind: Scans 2588, 2589, 2590; Background Corrected with Scan 2581

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	19.3	10257	PASS
68	69	0.00	2	0.9	101	PASS
69	198	0.00	100	21.6	11436	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	32.1	17001	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	53008	PASS
199	198	5	9	6.4	3379	PASS
275	198	10	60	32.5	17228	PASS
365	198	1	100	3.7	1966	PASS
441	442	0.01	24	16.2	6536	PASS
442	198	50	100	76.1	40341	PASS
443	442	15	24	19.2	7733	PASS