
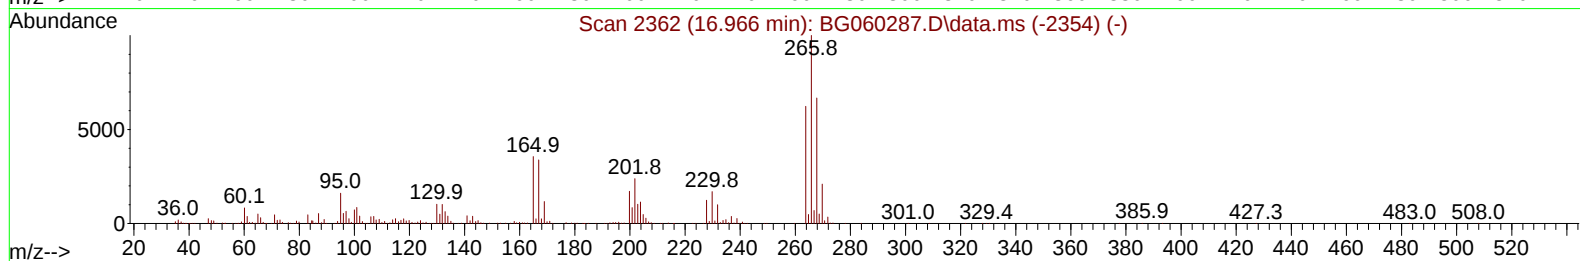
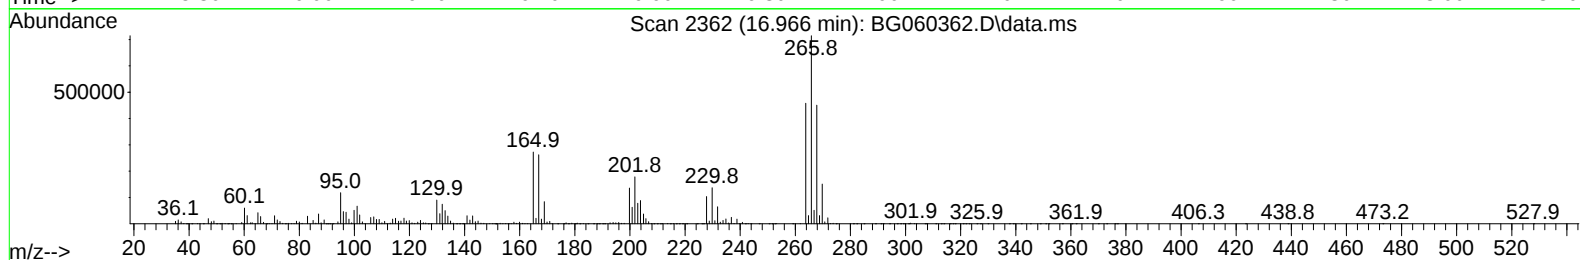


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011924\
Data File : BG060362.D
Acq On : 19 Jan 2024 9:21
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 19 10:23:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration

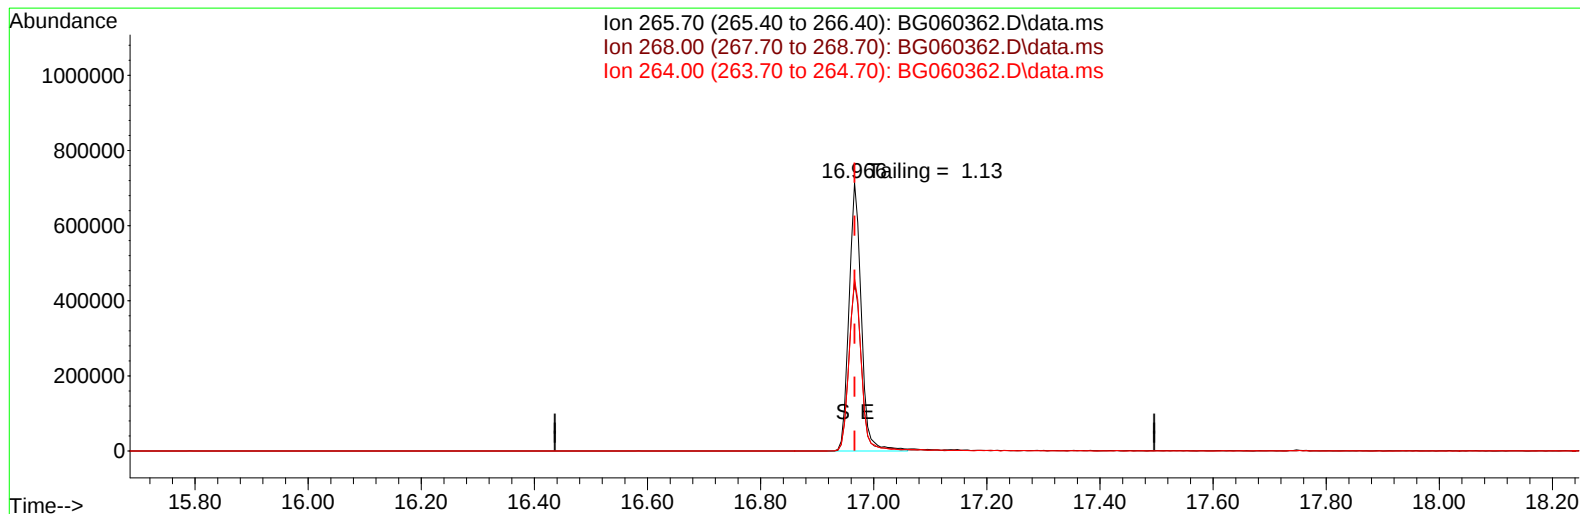

TIC: BG060362.D\data.ms

(70) Pentachlorophenol (C)




16.966min (-0.000) 27748.40 ng m

response 1083779

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	71.80	63.05
264.00	62.30	64.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011924\
Data File : BG060362.D
Acq On : 19 Jan 2024 9:21
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 19 10:23:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration

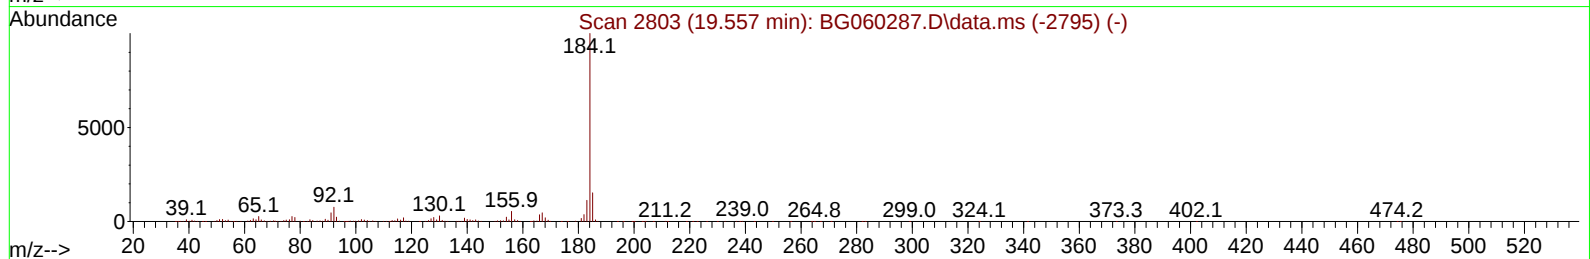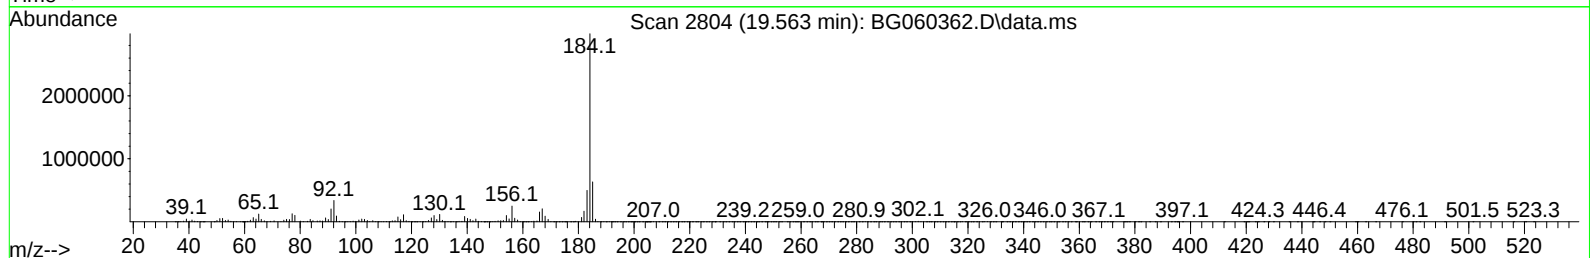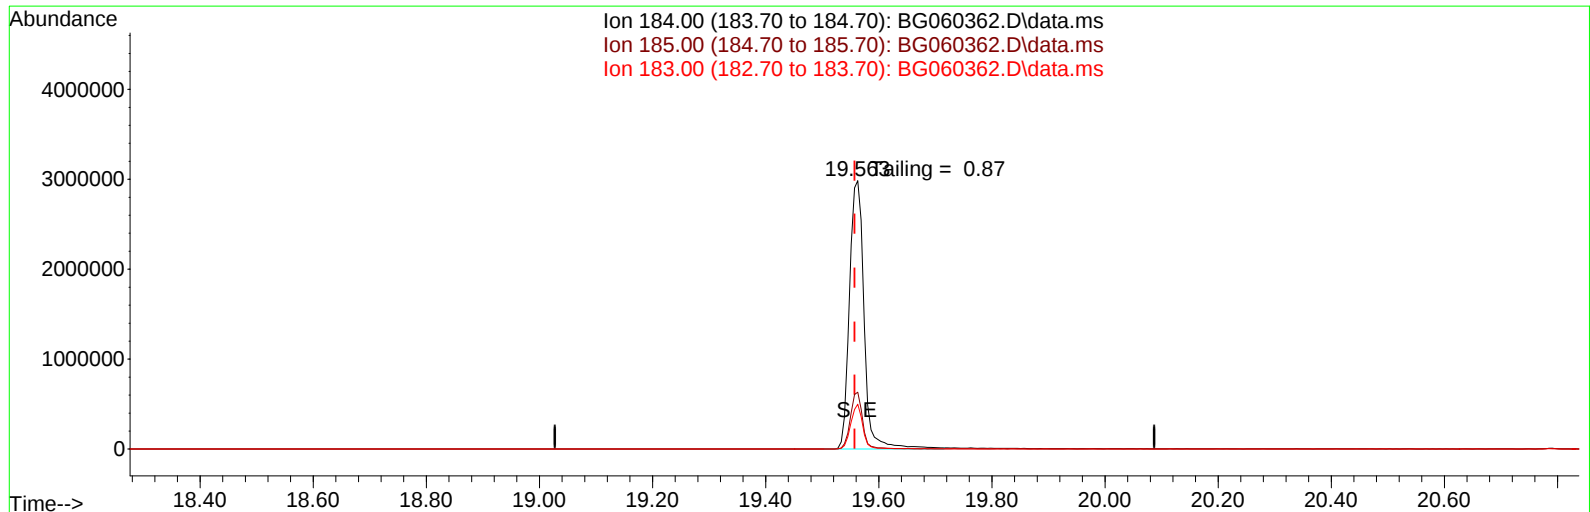

TIC: BG060362.D\data.ms

(77) Benzidine**19.563min (+ 0.006) 614753.93 ng****response 5382329**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	21.17#
183.00	11.20	16.69#
0.00	0.00	0.00