

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011924\
 Data File : BG060373.D
 Acq On : 19 Jan 2024 17:41
 Operator : MA/JU
 Sample : P1183-01 2X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MR-305-0-2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG060373.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.640	91	94	105	rVB3	27491	53082	1.29%	0.140%
2	4.121	170	176	180	rBV	30422	52482	1.27%	0.139%
3	5.038	325	332	337	rBV2	41823	70647	1.71%	0.187%
4	5.502	403	411	423	rBV	1378114	2366985	57.36%	6.249%
5	7.094	674	682	697	rBV	1319546	2370023	57.43%	6.257%
6	7.929	815	824	832	rBV	926669	1563595	37.89%	4.128%
7	9.092	1012	1022	1032	rBV	773407	1427330	34.59%	3.768%
8	9.644	1106	1116	1120	rBV7	21150	42659	1.03%	0.113%
9	10.731	1294	1301	1320	rBV	1196518	2188116	53.02%	5.777%
10	11.472	1420	1427	1430	rBV3	26347	48988	1.19%	0.129%
11	13.187	1712	1719	1730	rBV	2314948	3578195	86.71%	9.446%
12	14.568	1946	1954	1961	rBV	2110840	3308799	80.18%	8.735%
13	14.633	1961	1965	1971	rVB2	33605	57179	1.39%	0.151%
14	14.774	1982	1989	1995	rBV2	26928	62026	1.50%	0.164%
15	15.620	2128	2133	2136	rBV3	29073	43618	1.06%	0.115%
16	16.054	2201	2207	2216	rBV	1804069	2784639	67.48%	7.351%
17	17.318	2416	2422	2426	rBV	2506319	3817625	92.51%	10.079%
18	17.353	2426	2428	2435	rVB	244959	362664	8.79%	0.957%
19	18.199	2568	2572	2576	rBV2	193647	305451	7.40%	0.806%
20	19.374	2767	2772	2777	rBV	646245	925252	22.42%	2.443%
21	19.733	2830	2833	2841	rVB	593875	875037	21.20%	2.310%
22	19.932	2862	2867	2872	rBV	3313979	4126806	100.00%	10.895%
23	21.583	3142	3148	3153	rBV2	2162485	3679307	89.16%	9.713%
24	24.756	3682	3688	3707	rVB	1191525	3768214	91.31%	9.948%




Sum of corrected areas: 37878719

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011924\
Data File : BG060373.D
Acq On : 19 Jan 2024 17:41
Operator : MA/JU
Sample : P1183-01 2X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MR-305-0-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

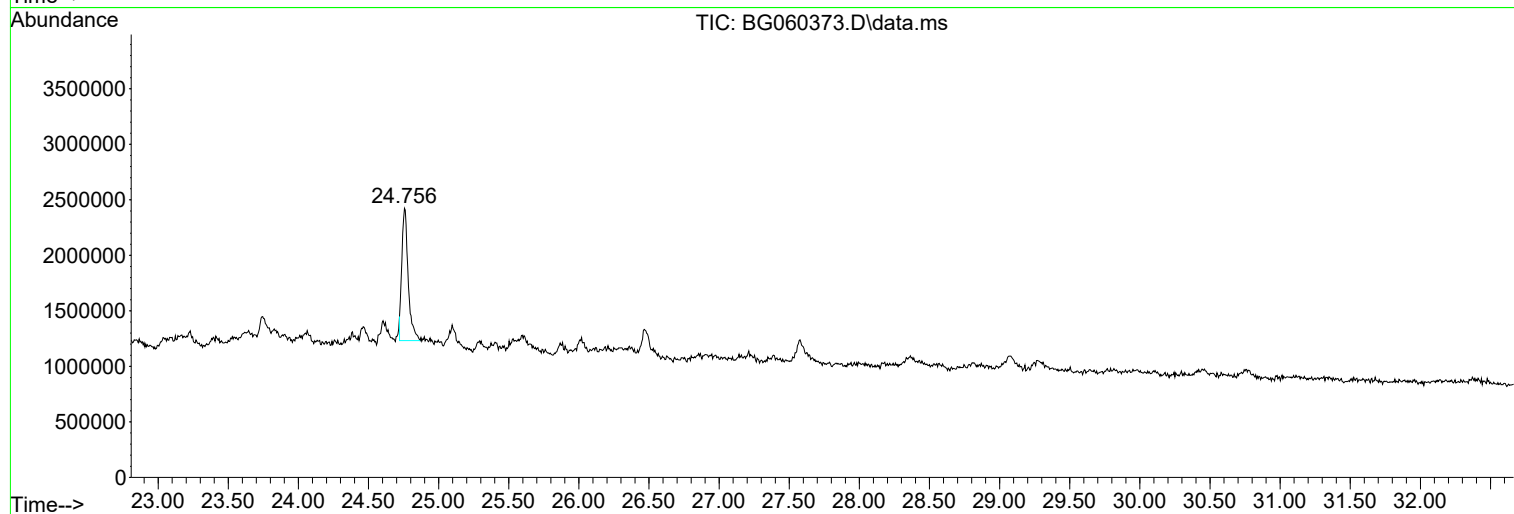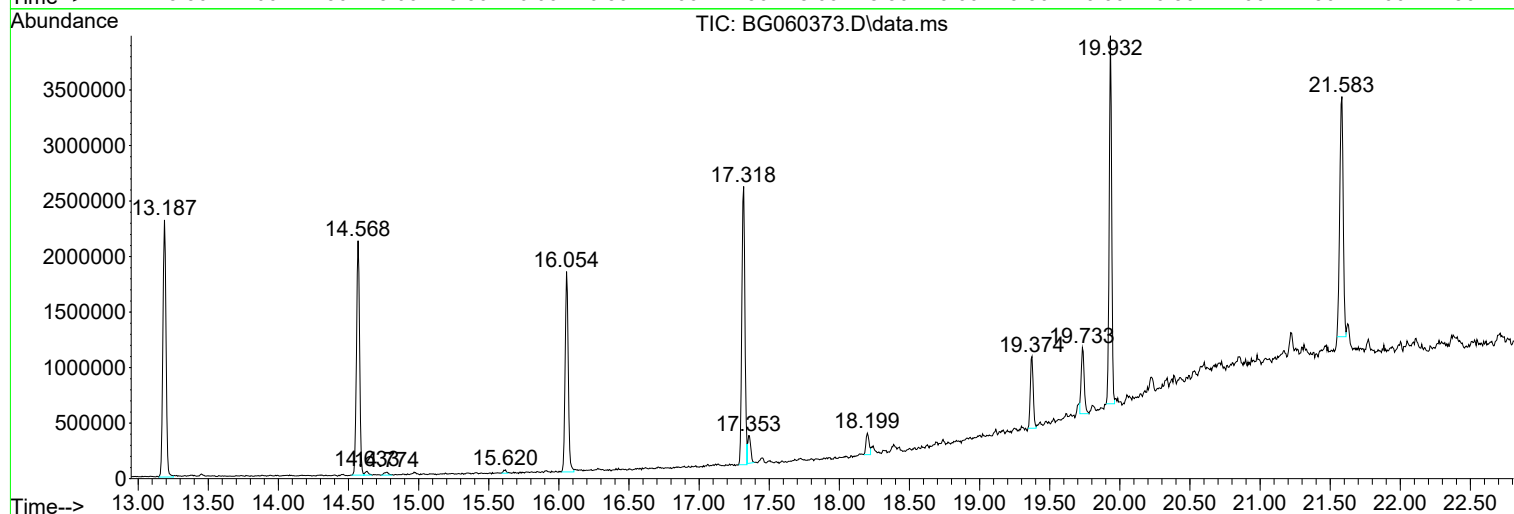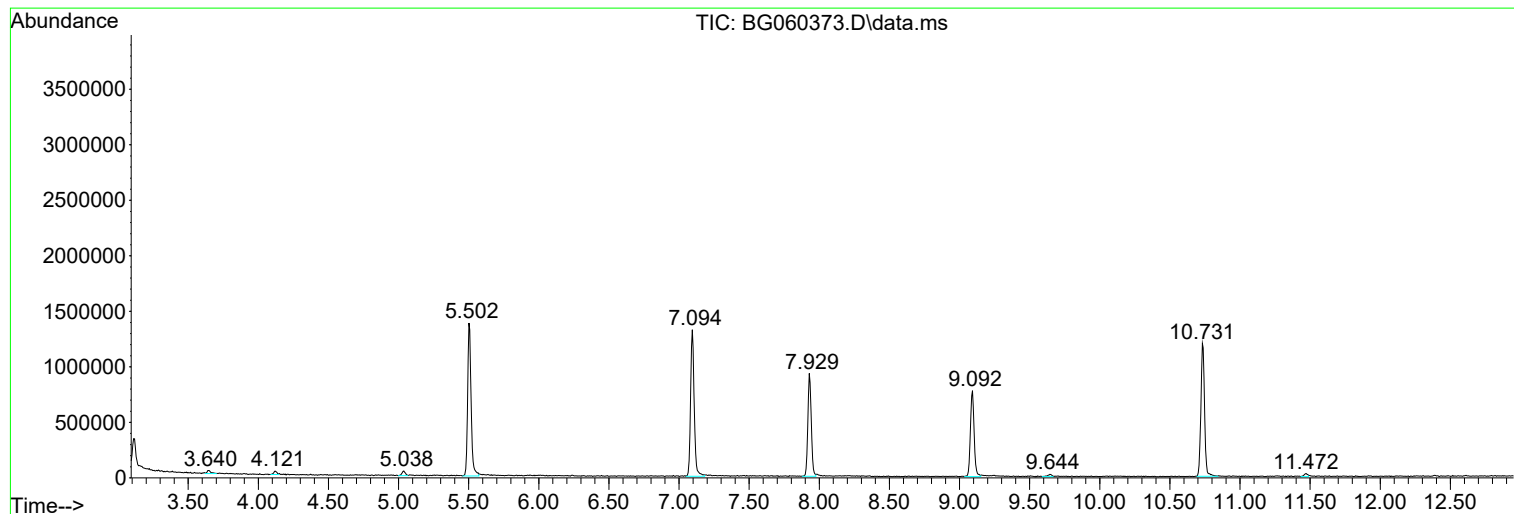

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011924\
Data File : BG060373.D
Acq On : 19 Jan 2024 17:41
Operator : MA/JU
Sample : P1183-01 2X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MR-305-0-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011924\
Data File : BG060373.D
Acq On : 19 Jan 2024 17:41
Operator : MA/JU
Sample : P1183-01 2X
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MR-305-0-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------