


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011924\
Data File : BG060362.D
Acq On : 19 Jan 2024 9:21
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jan 09 04:07:12 2024

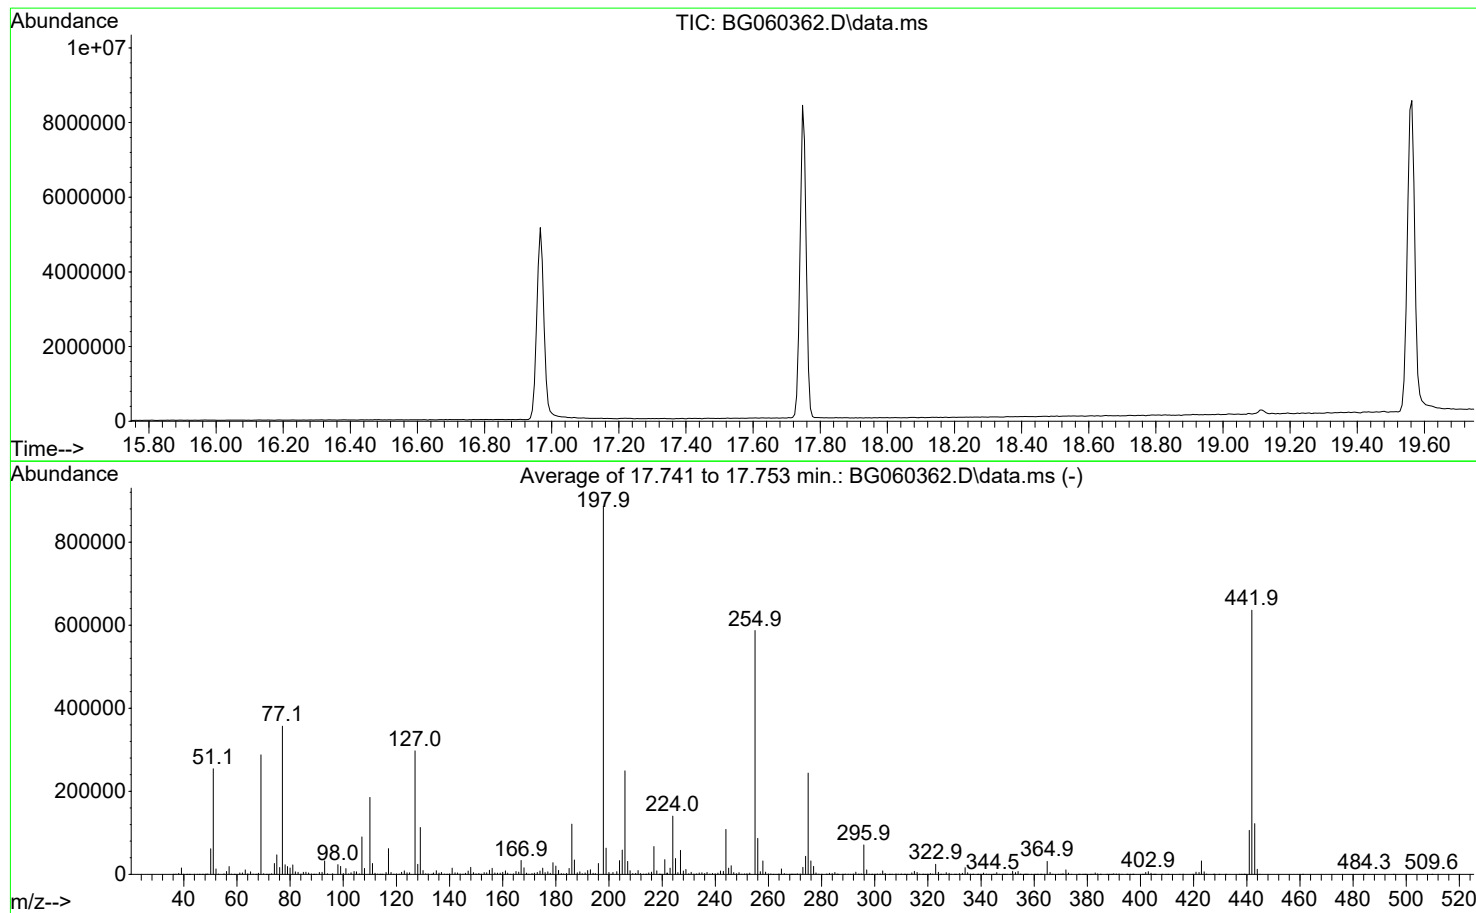

AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2486

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.7	254208	PASS
68	69	0.00	2	0.9	2687	PASS
69	198	0.00	100	32.5	287800	PASS
70	69	0.00	2	0.6	1623	PASS
127	198	10	80	33.6	297621	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	885760	PASS
199	198	5	9	7.1	63296	PASS
275	198	10	60	27.5	243831	PASS
365	198	1	100	3.5	31267	PASS
441	198	0.01	100	11.9	105843	PASS
442	442	50	100	100.0	636181	PASS
443	442	15	24	19.2	122158	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
1/19/2024	BNA_G	<u>BG060362.D</u>
Compound Name	Response	Retention Time
DDT	2704182	20.791
DDD	68687	20.344
DDE	5079	19.845
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
73766	2777948	2.66

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011924\
Data File : BG060362.D
Acq On : 19 Jan 2024 9:21
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 19 10:23:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration

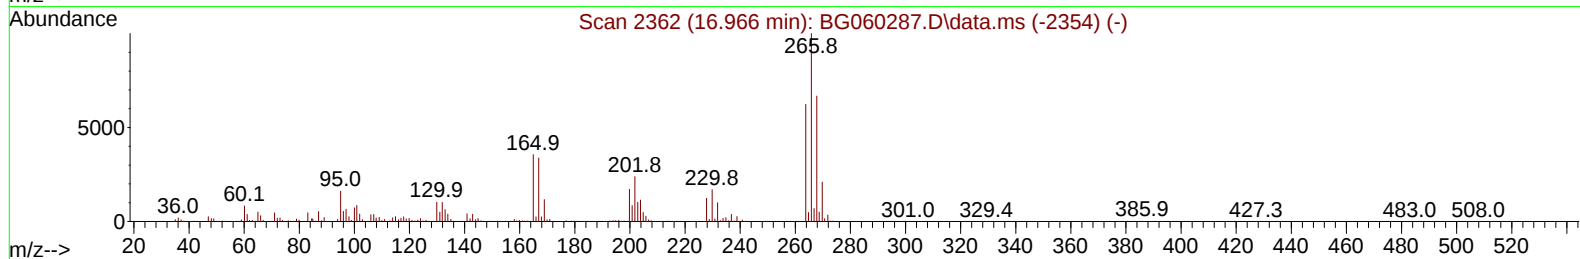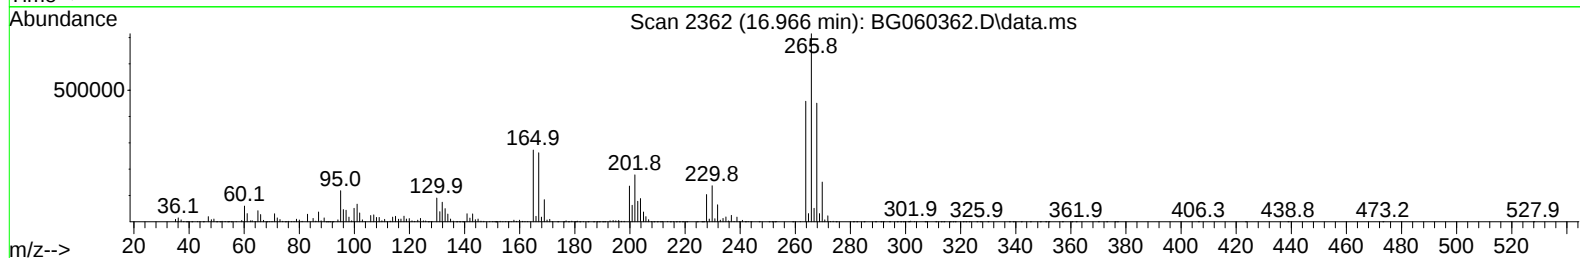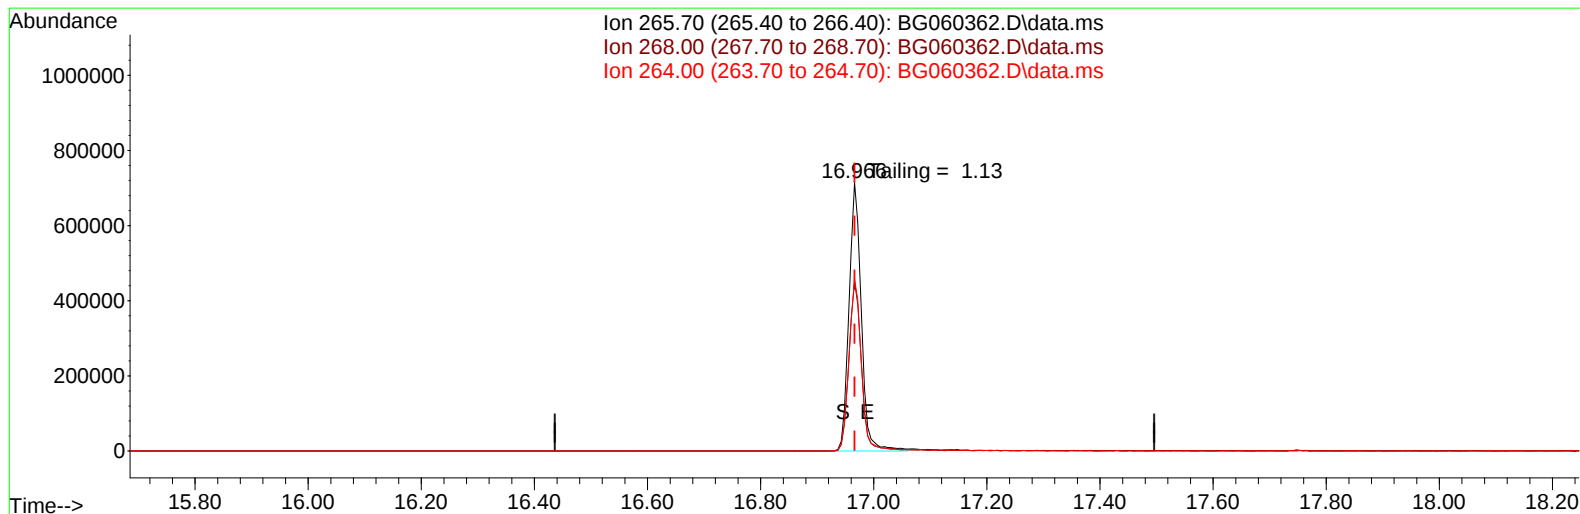

TIC: BG060362.D\data.ms

(70) Pentachlorophenol (C)

16.966min (-0.000) 27748.40 ng m




response 1083779

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	71.80	63.05
264.00	62.30	64.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG011924\
Data File : BG060362.D
Acq On : 19 Jan 2024 9:21
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 19 10:23:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 09 04:07:12 2024
Response via : Initial Calibration

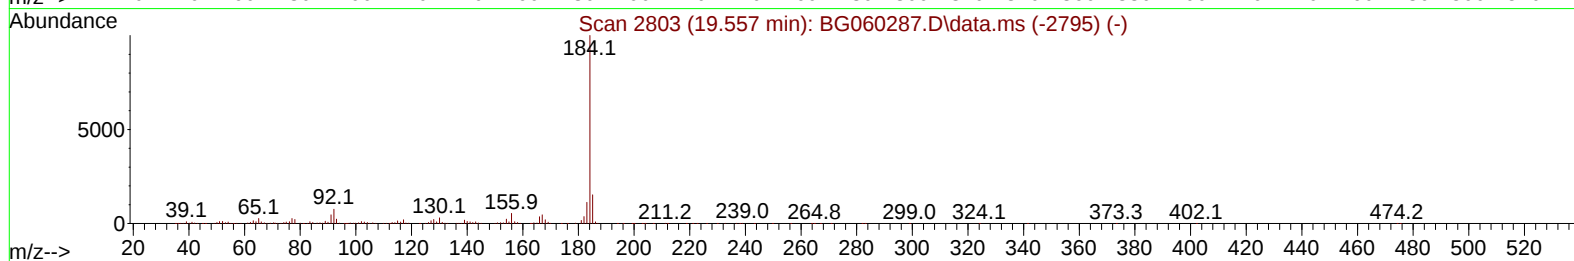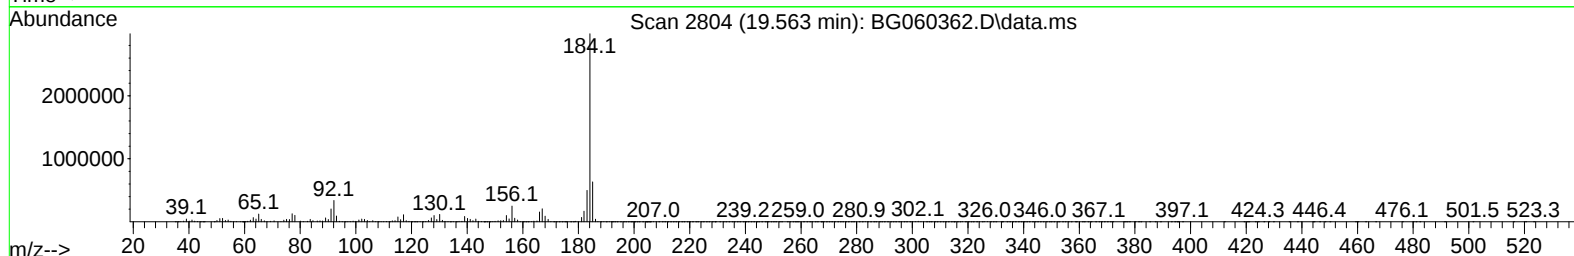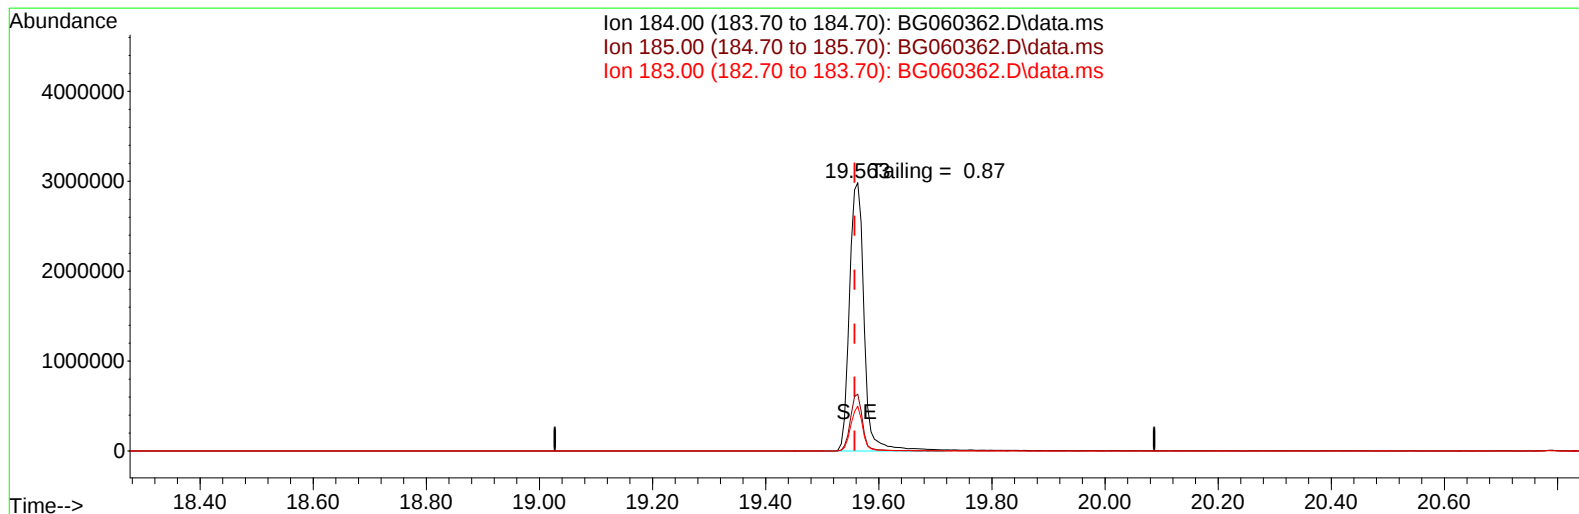

TIC: BG060362.D\data.ms

(77) Benzidine

19.563min (+ 0.006) 614753.93 ng

response 5382329

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	21.17#
183.00	11.20	16.69#
0.00	0.00	0.00