


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG012015\
 Data File : BG015886.D
 Acq On : 20 Jan 2015 11:05
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG012015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 20 17:47:40 2015

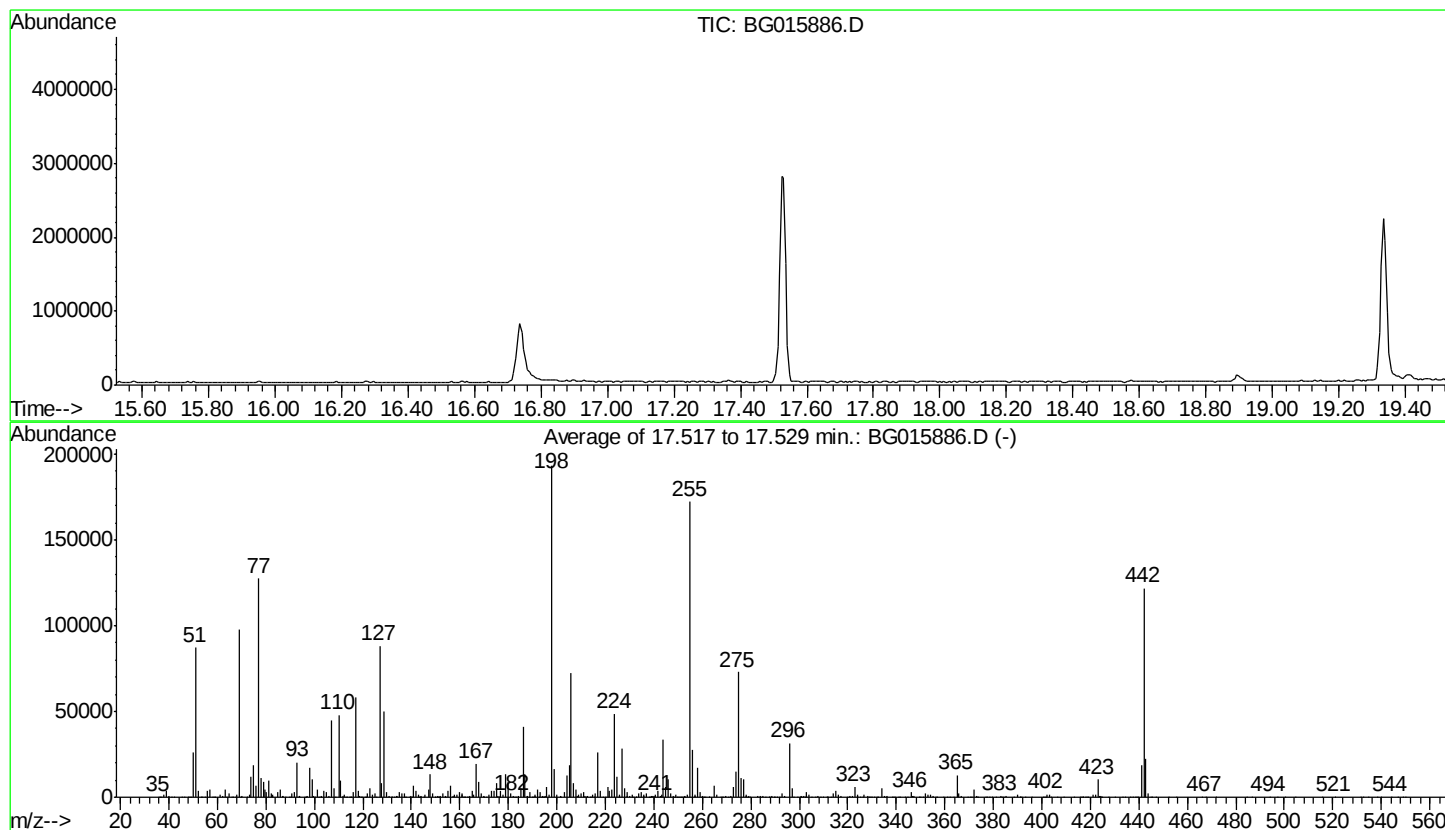

AutoFind: Scans 2524, 2525, 2526; Background Corrected with Scan 2518

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.1	87242	PASS
68	69	0.00	2	1.7	1666	PASS
69	198	0.00	100	50.4	97491	PASS
70	69	0.00	2	0.4	425	PASS
127	198	10	80	45.7	88357	PASS
197	198	0.00	2	0.7	1373	PASS
198	198	100	100	100.0	193314	PASS
199	198	5	9	8.5	16414	PASS
275	198	10	60	37.8	73058	PASS
365	198	1	100	6.6	12835	PASS
441	442	0.01	24	15.1	18434	PASS
442	198	50	100	63.1	121992	PASS
443	442	15	24	18.5	22628	PASS