
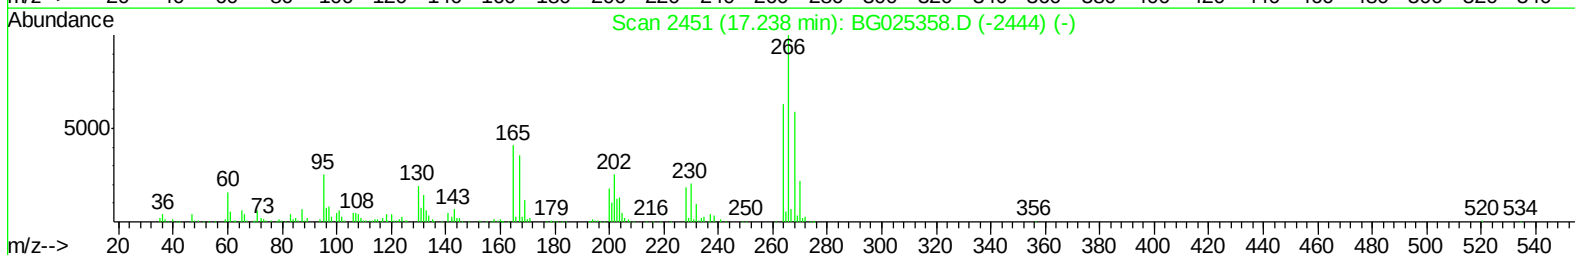
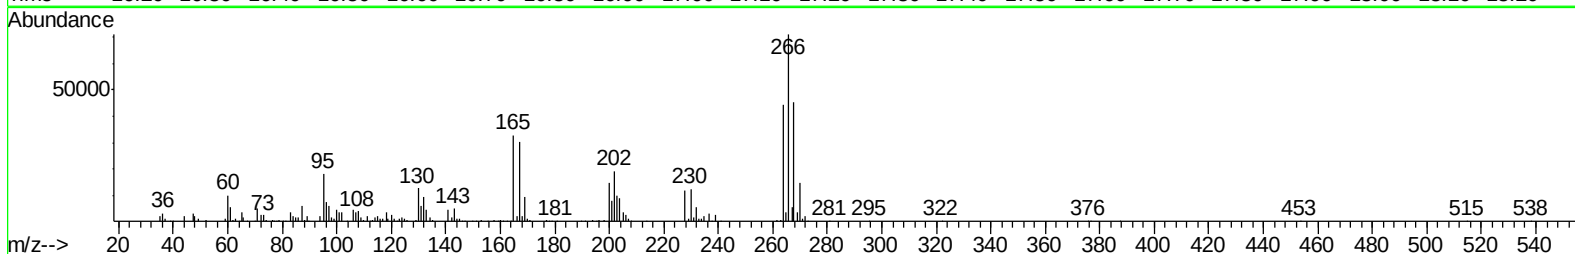


Data Path : Z:\HPCHEM1\BNA_G\Data\BG012017\
Data File : BG025533.D
Acq On : 20 Jan 2017 11:19
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 23 07:52:57 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 10 11:26:22 2017
Response via : Initial Calibration

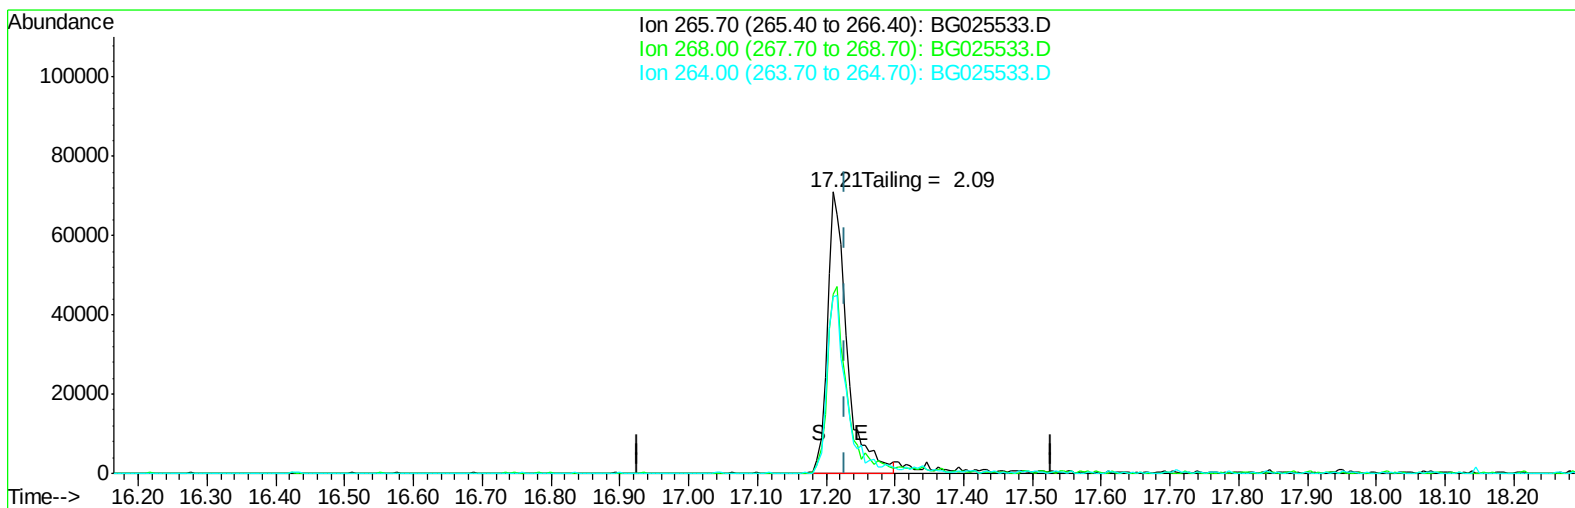

TIC: BG025533.D

(69) Pentachlorophenol (C)




17.210min (-0.017) 196242.18ng

response 139707

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	63.82
264.00	62.60	62.59
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG012017\
 Data File : BG025533.D
 Acq On : 20 Jan 2017 11:19
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 23 07:52:57 2017
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG122116.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 10 11:26:22 2017
 Response via : Initial Calibration

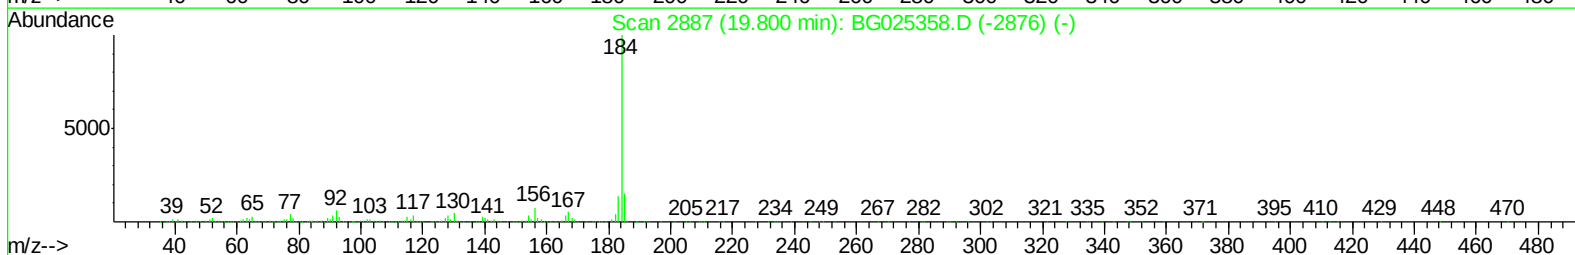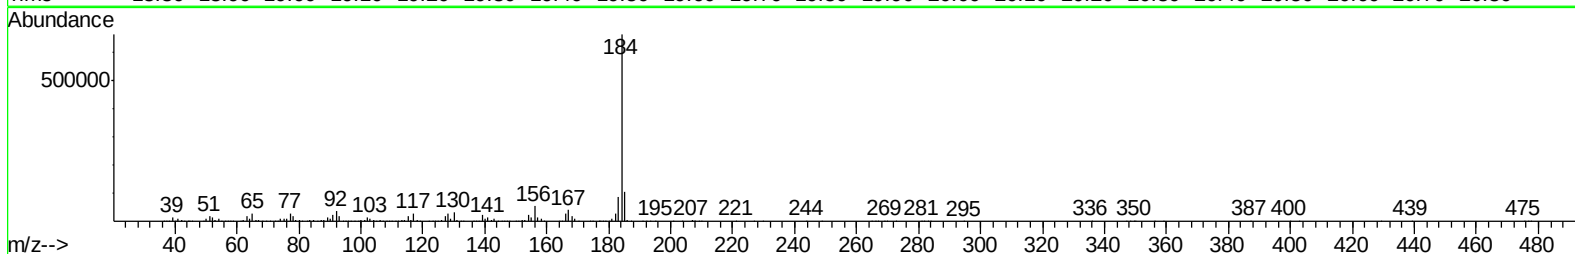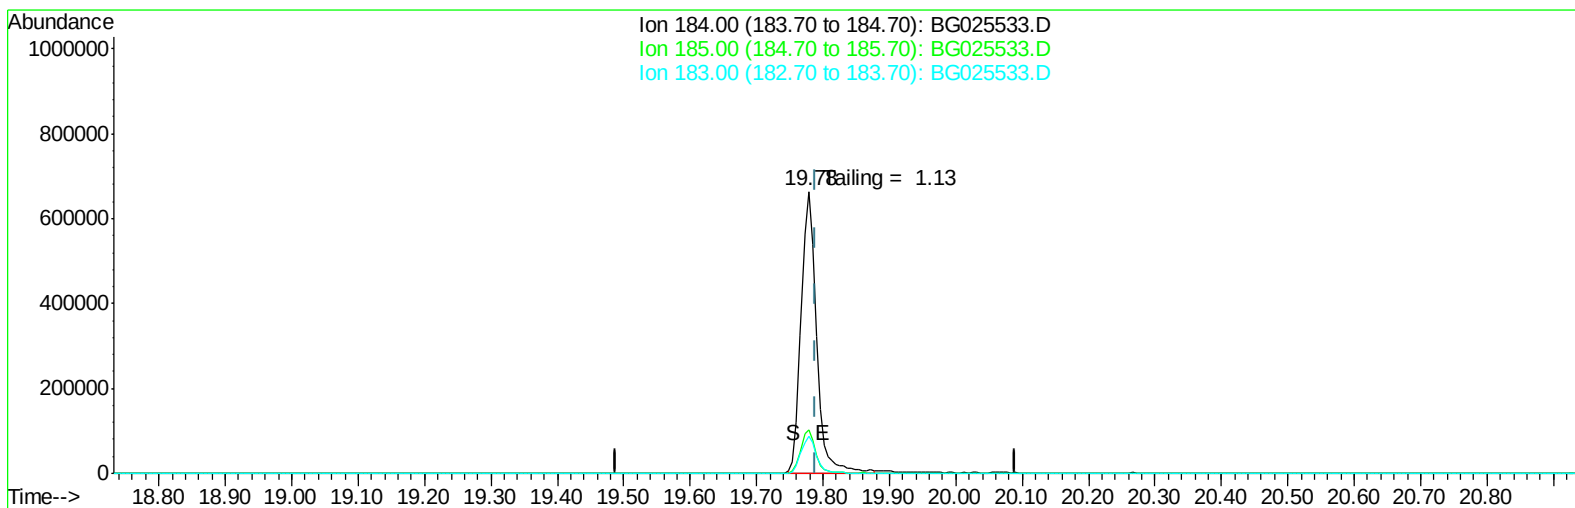

TIC: BG025533.D

(76) Benzidine

19.778min (-0.011) 360176.13ng

response 1069149

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	15.68
183.00	13.80	13.00
0.00	0.00	0.00