
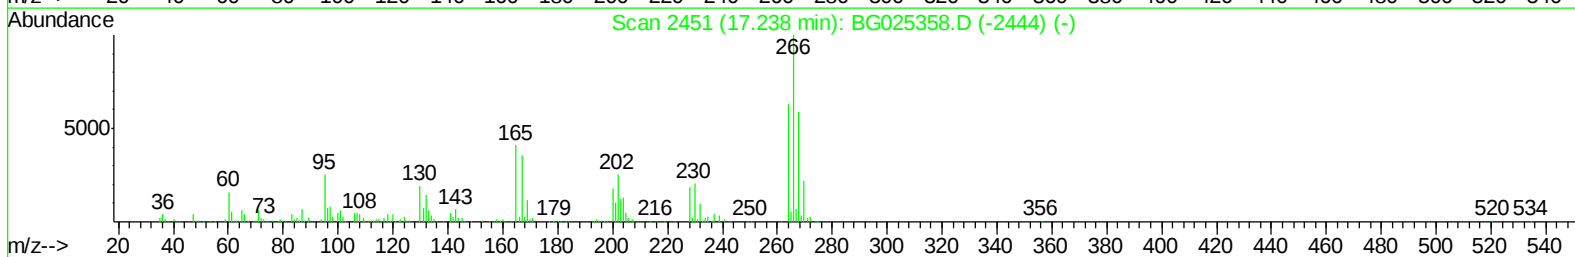
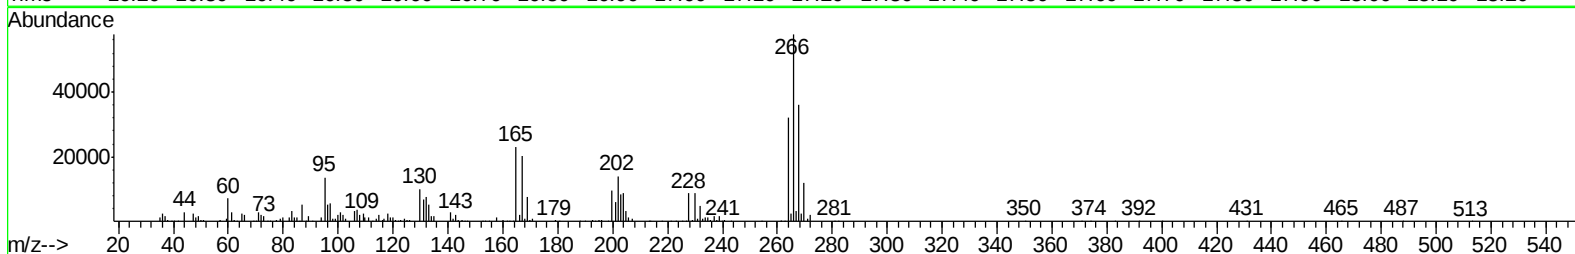


Data Path : Z:\HPCHEM1\BNA_G\Data\BG012017\
Data File : BG025550.D
Acq On : 20 Jan 2017 23:23
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 23 07:53:38 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 10 11:26:22 2017
Response via : Initial Calibration

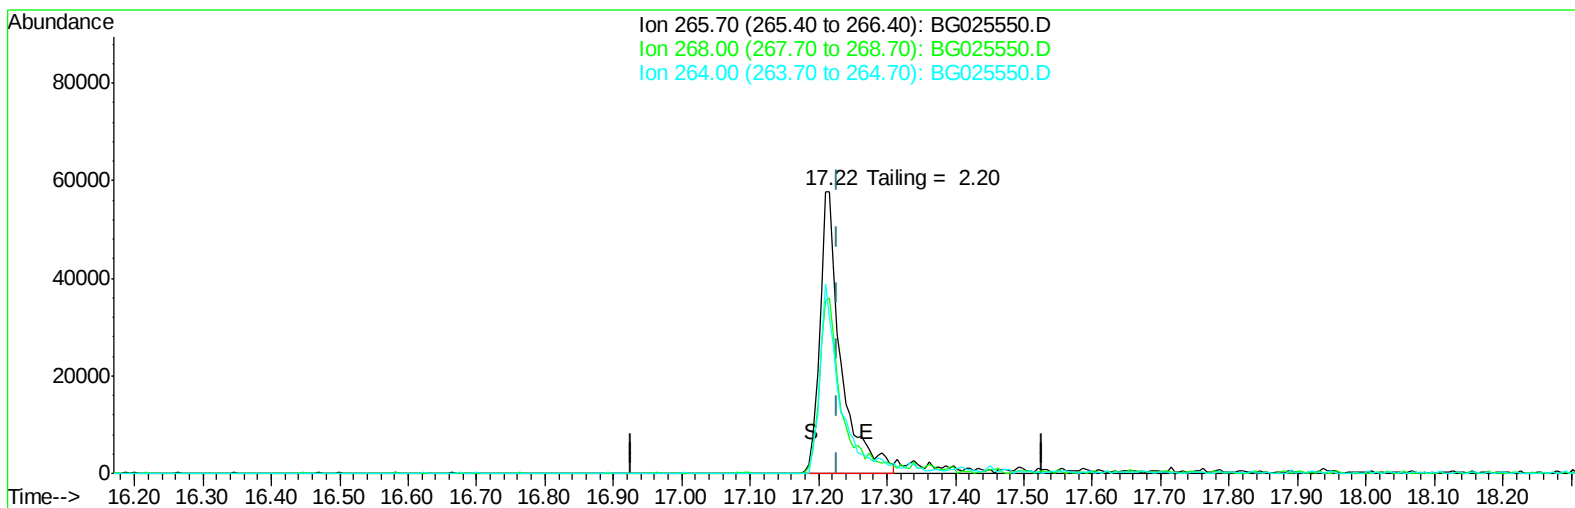

TIC: BG025550.D

(69) Pentachlorophenol (C)




17.216min (-0.012) 243923.93ng

response 125316

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	62.48
264.00	62.60	55.54
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG012017\
Data File : BG025550.D
Acq On : 20 Jan 2017 23:23
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 23 07:53:38 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG122116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 10 11:26:22 2017
Response via : Initial Calibration

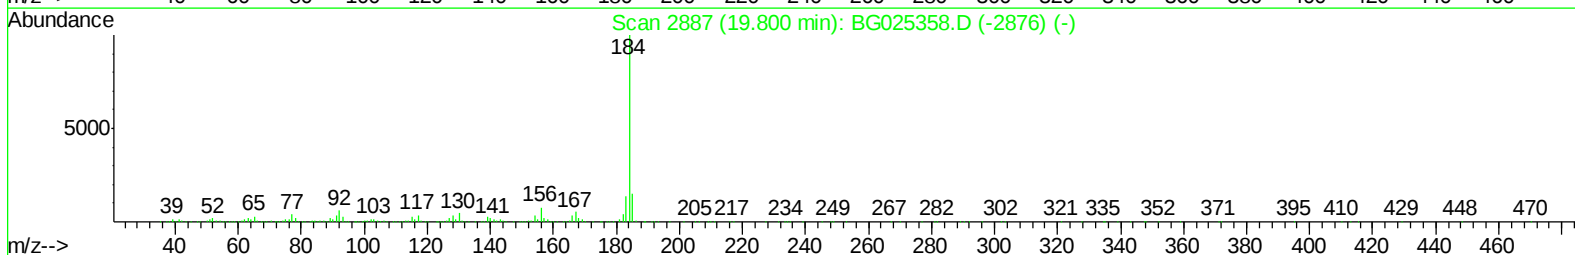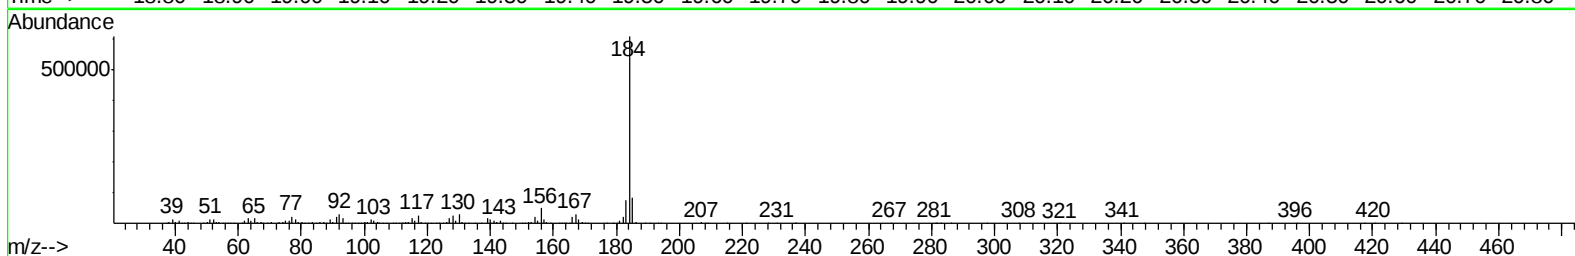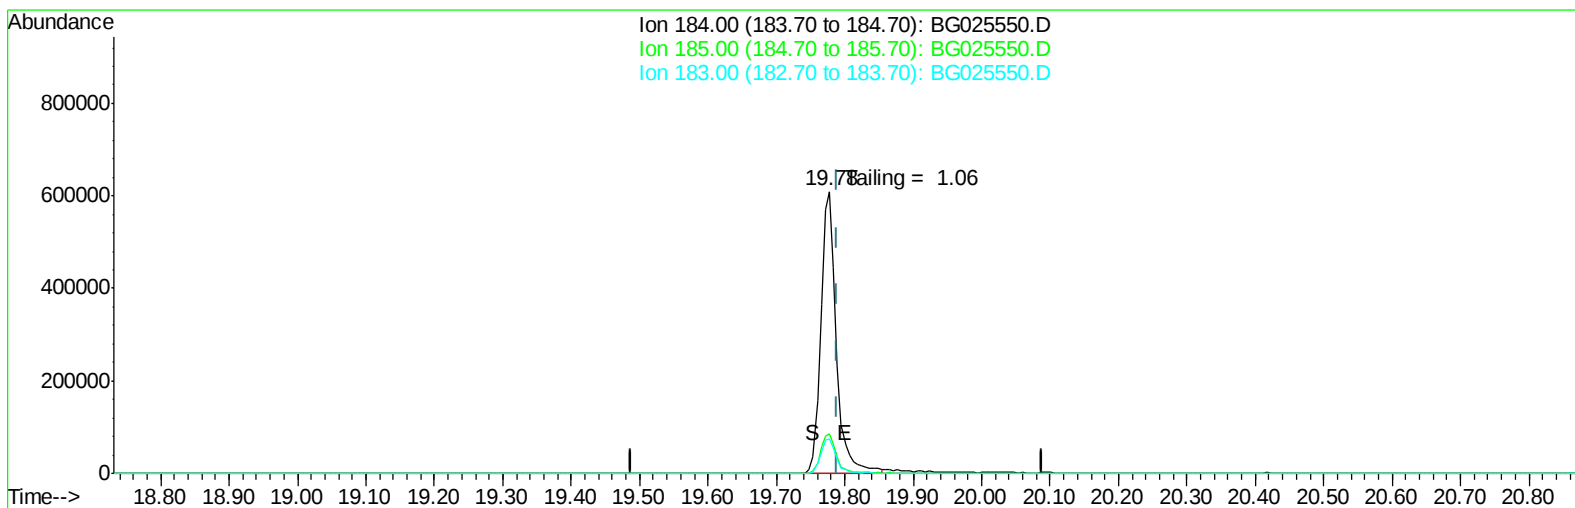

TIC: BG025550.D

(76) Benzidine

19.777min (-0.012) 254286.21ng

response 976832

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	14.03
183.00	13.80	12.29
0.00	0.00	0.00