


Data Path : Z:\HPCHEM1\BNA G\DATA\BG012017\
 Data File : BG025550.D
 Acq On : 20 Jan 2017 23:23
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG122116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 10 11:26:22 2017

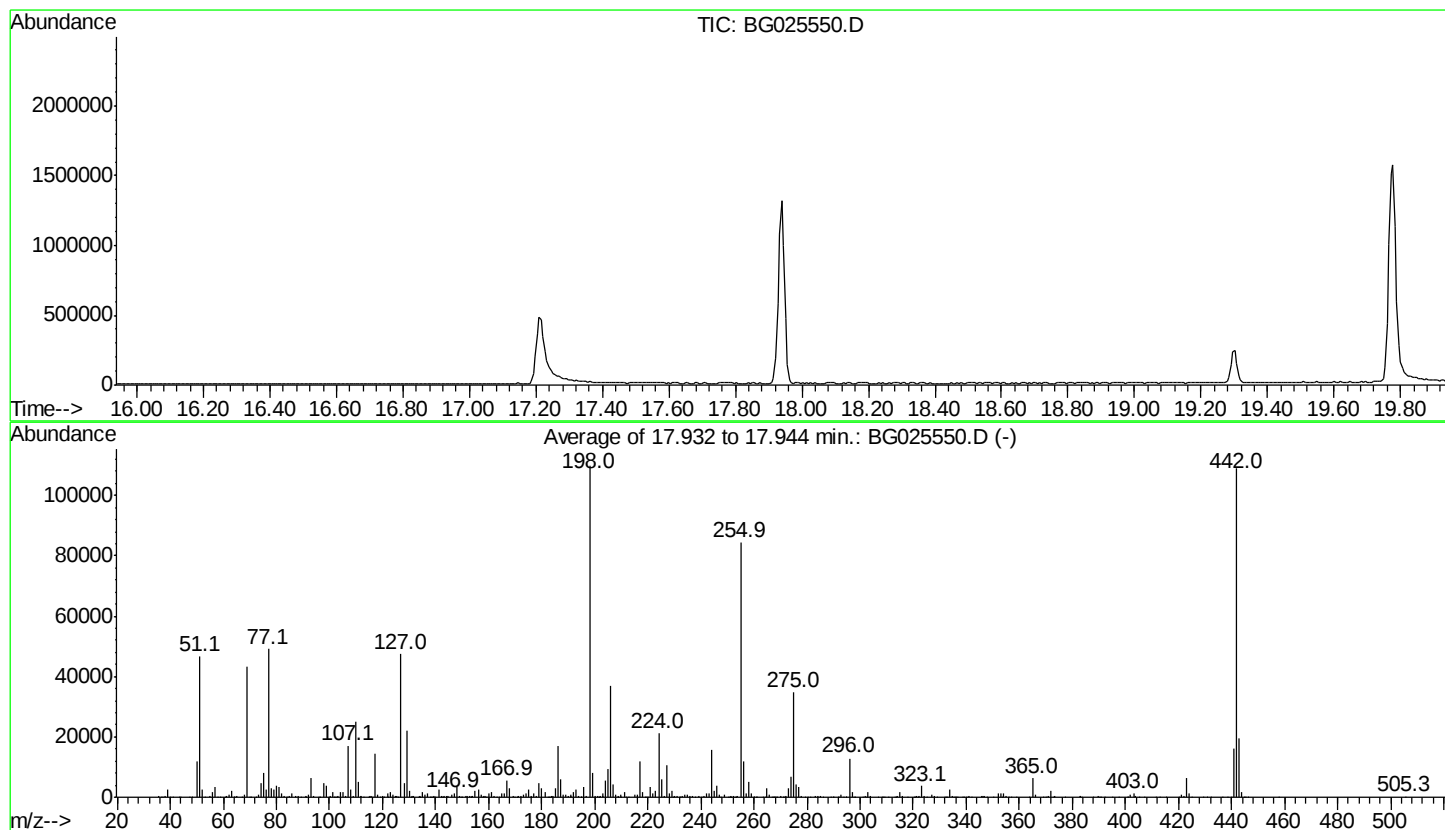

AutoFind: Scans 2569, 2570, 2571; Background Corrected with Scan 2562

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.4	46586	PASS
68	69	0.00	2	1.6	701	PASS
69	198	0.00	100	39.4	43314	PASS
70	69	0.00	2	0.4	161	PASS
127	198	10	80	43.1	47418	PASS
197	198	0.00	2	0.3	382	PASS
198	198	100	100	100.0	109914	PASS
199	198	5	9	7.4	8087	PASS
275	198	10	60	31.5	34597	PASS
365	198	1	100	5.7	6261	PASS
441	442	0.01	24	14.8	16167	PASS
442	198	50	100	99.2	109050	PASS
443	442	15	24	18.0	19576	PASS