
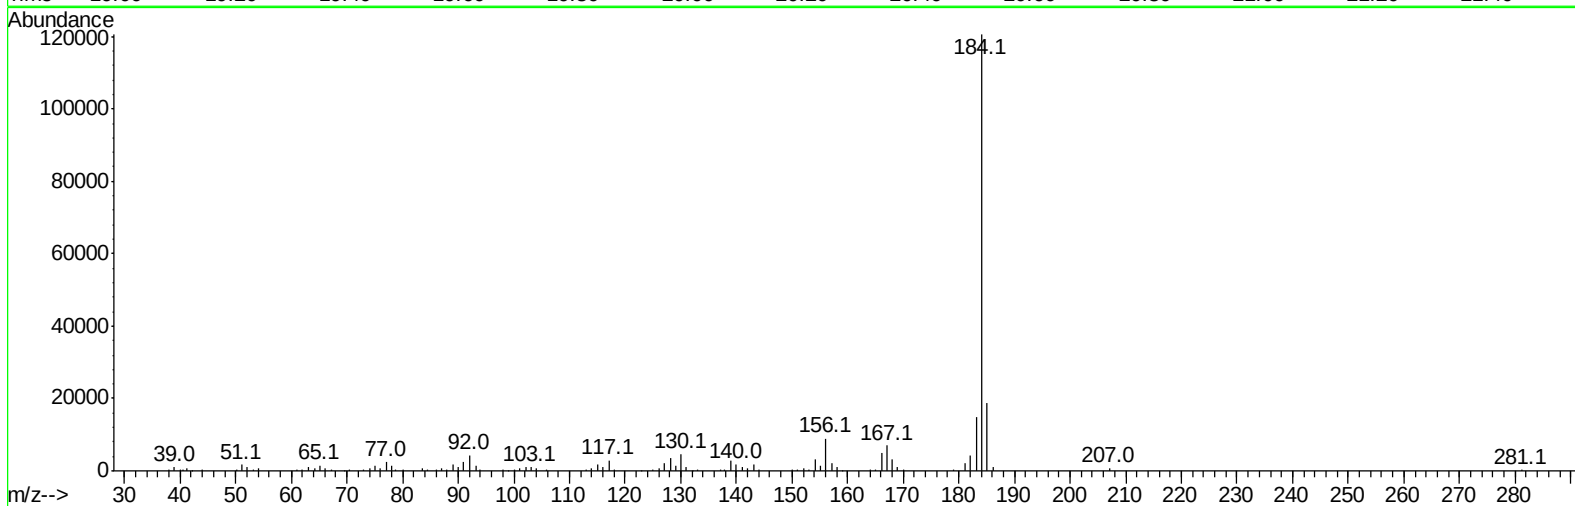


Data Path : U:\HPCHEM1\BNA G\DATA\BG012018\
Data File : BG032178.D
Acq On : 20 Jan 2018 13:41
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 22 06:37:54 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG011218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 18 10:13:16 2018
Response via : Initial Calibration

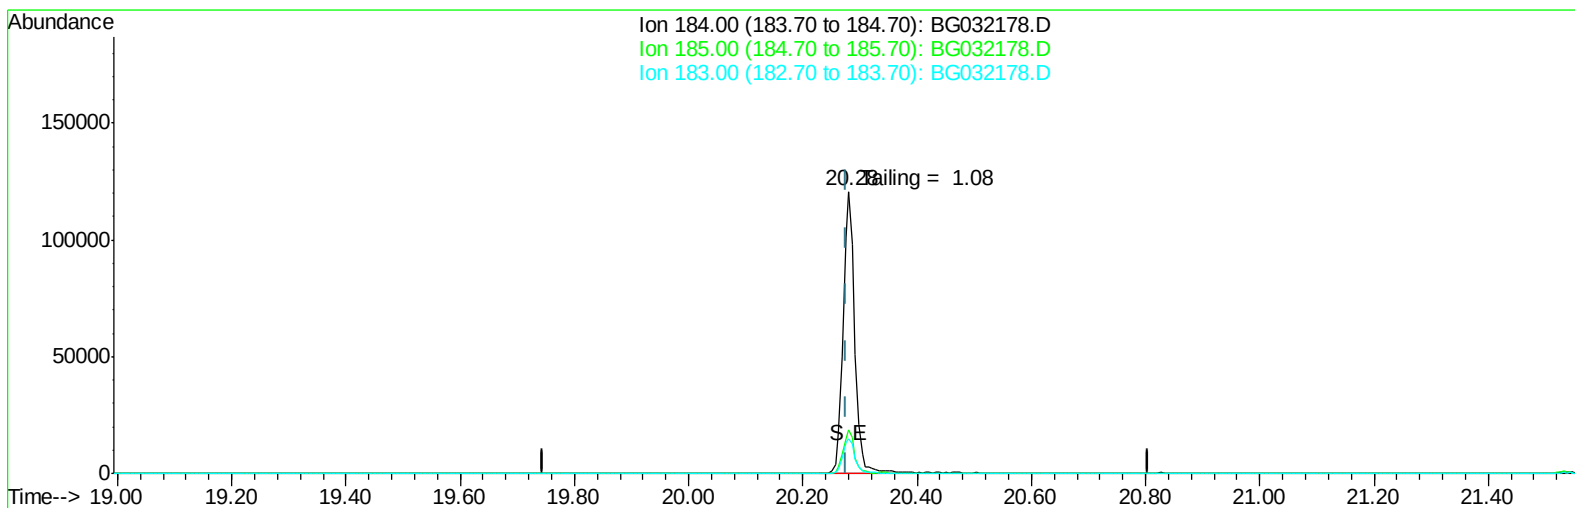

TIC: BG032178.D

(76) Benzidine



20.280min (+0.005) 116878.20ng

response 172438

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	15.53
183.00	13.30	12.43
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA G\DATA\BG012018\
Data File : BG032178.D
Acq On : 20 Jan 2018 13:41
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 22 06:37:54 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG011218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 18 10:13:16 2018
Response via : Initial Calibration

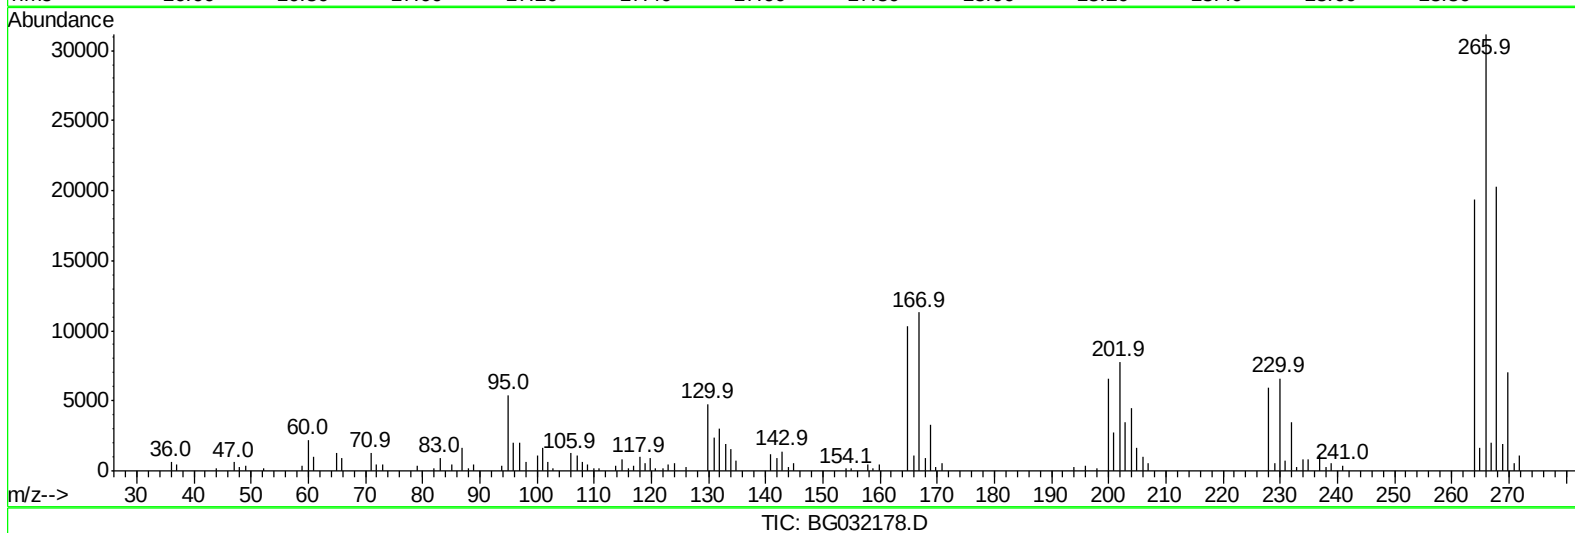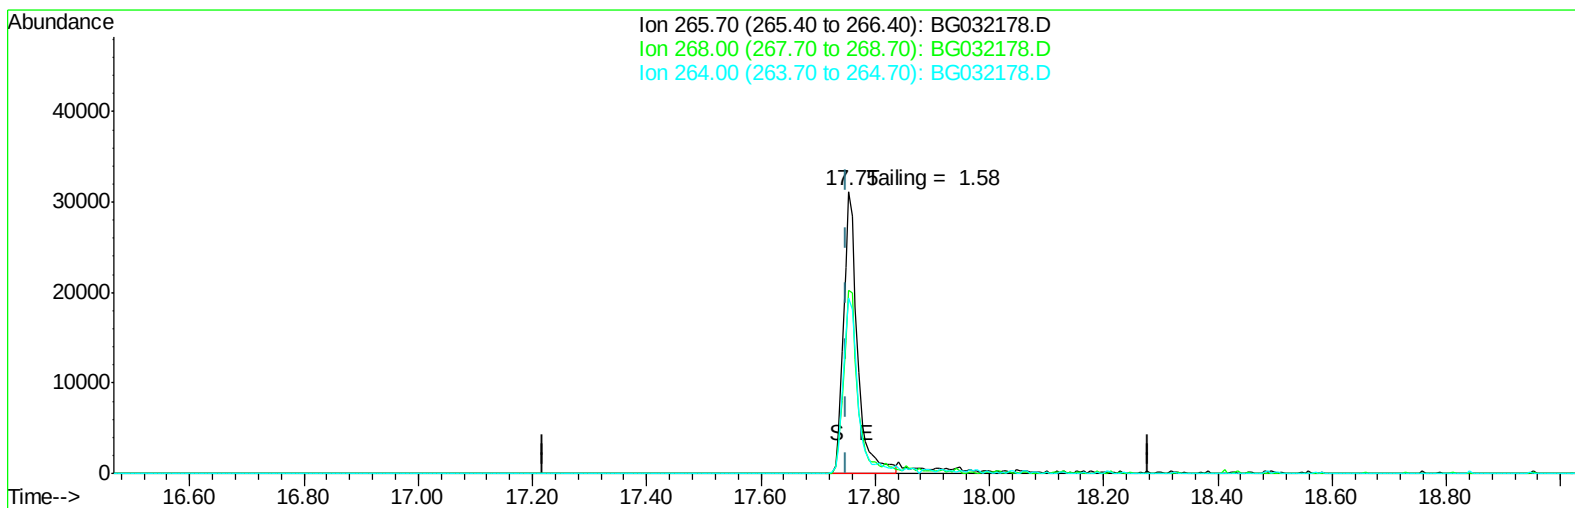

(69) Pentachlorophenol (C)

17.754min (+0.005) 12323.38ng

response 53565

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	65.01
264.00	62.00	62.29
0.00	0.00	0.00