
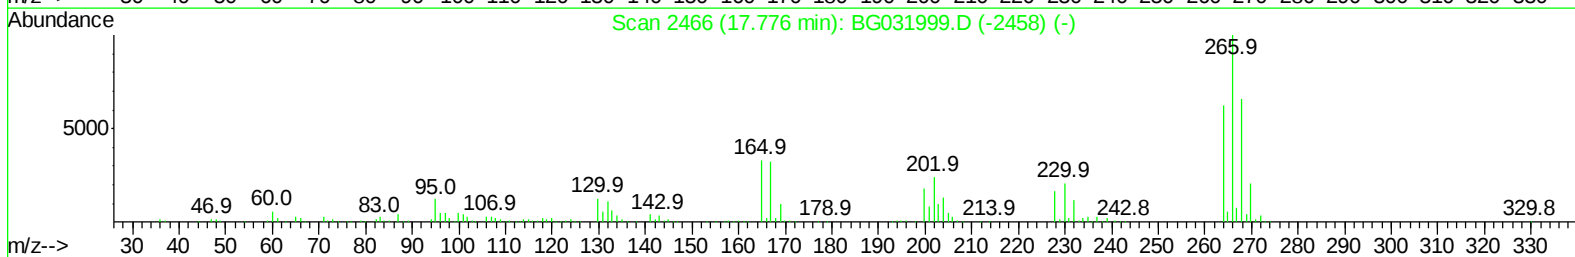
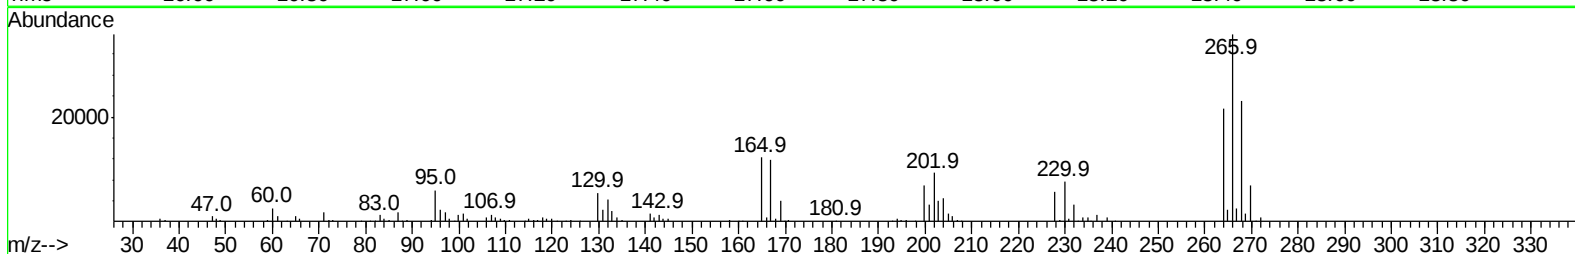


Data Path : U:\HPCHEM1\BNA G\DATA\BG012018\
Data File : BG032196.D
Acq On : 21 Jan 2018 2:12
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 22 06:40:01 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG011218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 18 10:13:16 2018
Response via : Initial Calibration

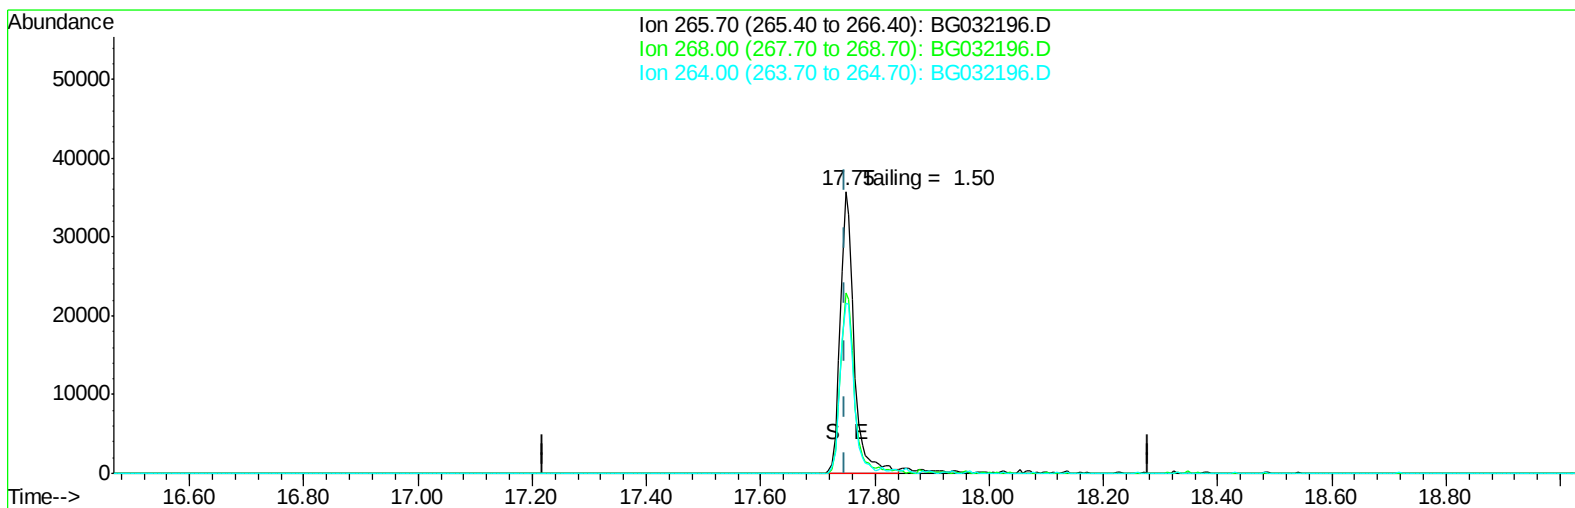

TIC: BG032196.D

(69) Pentachlorophenol (C)




17.748min (-0.001) 86840.37ng

response 60289

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.25
264.00	62.00	60.69
0.00	0.00	0.00

Data Path : U:\HPCHEM1\BNA G\DATA\BG012018\
 Data File : BG032196.D
 Acq On : 21 Jan 2018 2:12
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 22 06:40:01 2018
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG011218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 18 10:13:16 2018
 Response via : Initial Calibration

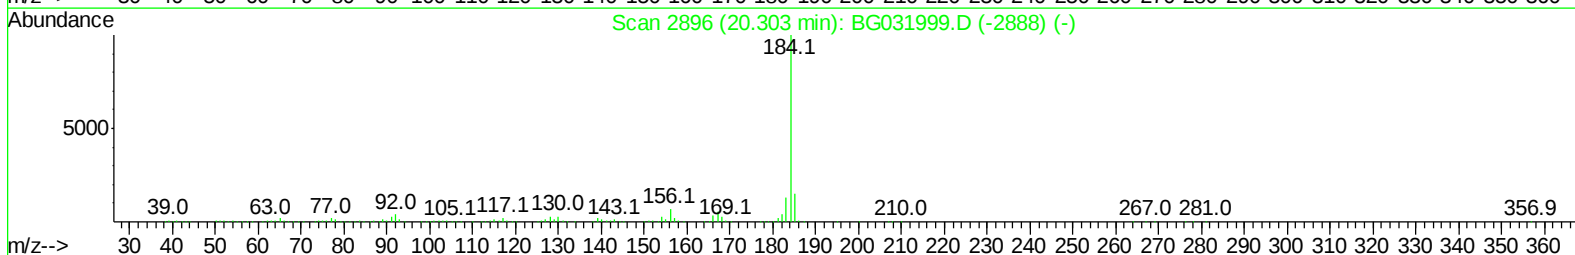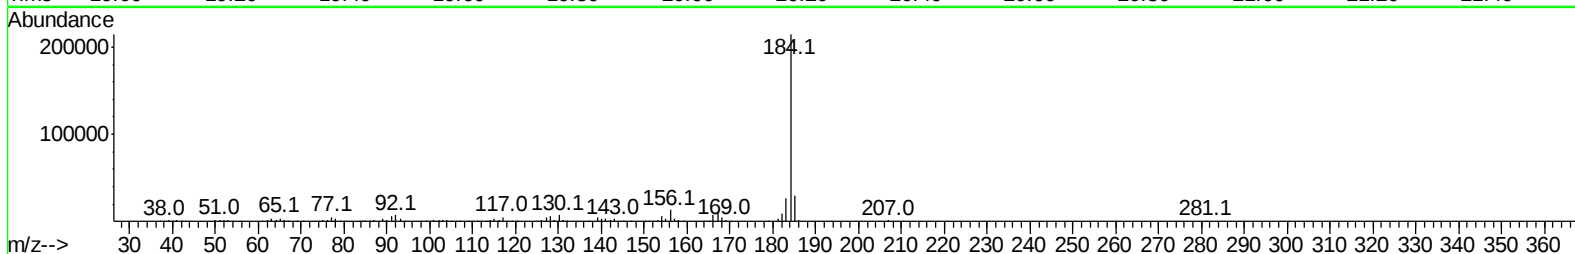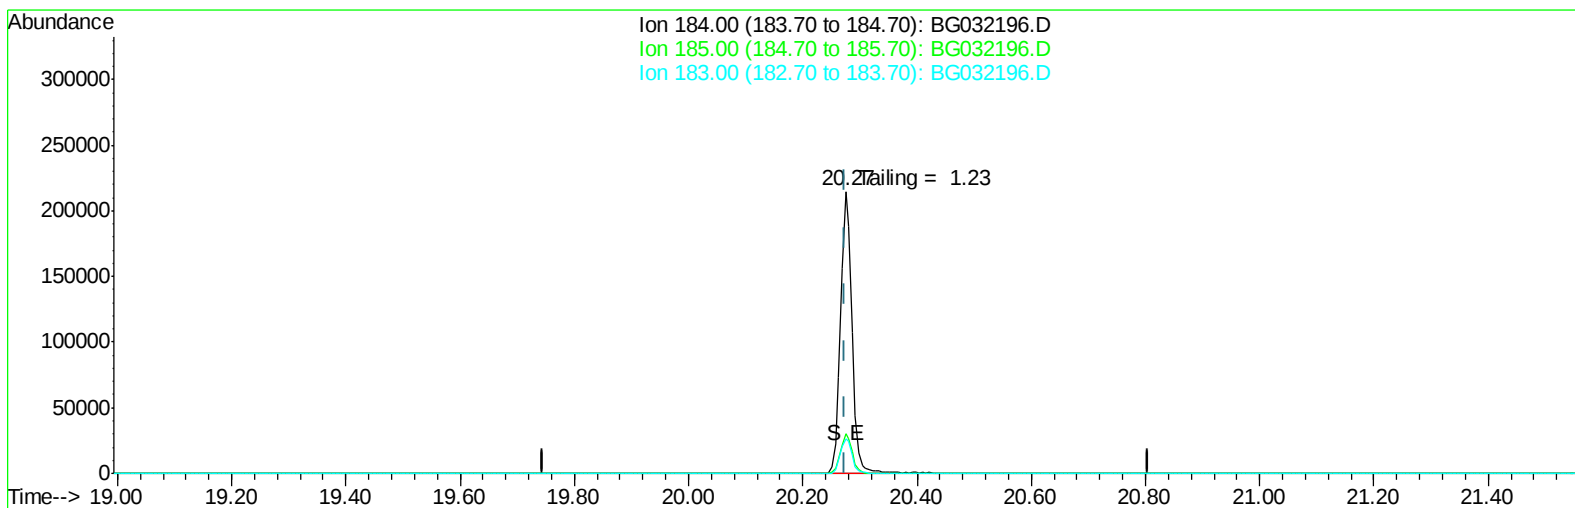

TIC: BG032196.D

(76) Benzidine

20.275min (-0.001) 155145.50ng

response 298729

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.06
183.00	13.30	12.19
0.00	0.00	0.00