


Data Path : Z:\HPCHEM1\BNA G\Data\BG012018\
 Data File : BG032178.D
 Acq On : 20 Jan 2018 13:41
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG011218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 18 10:13:16 2018

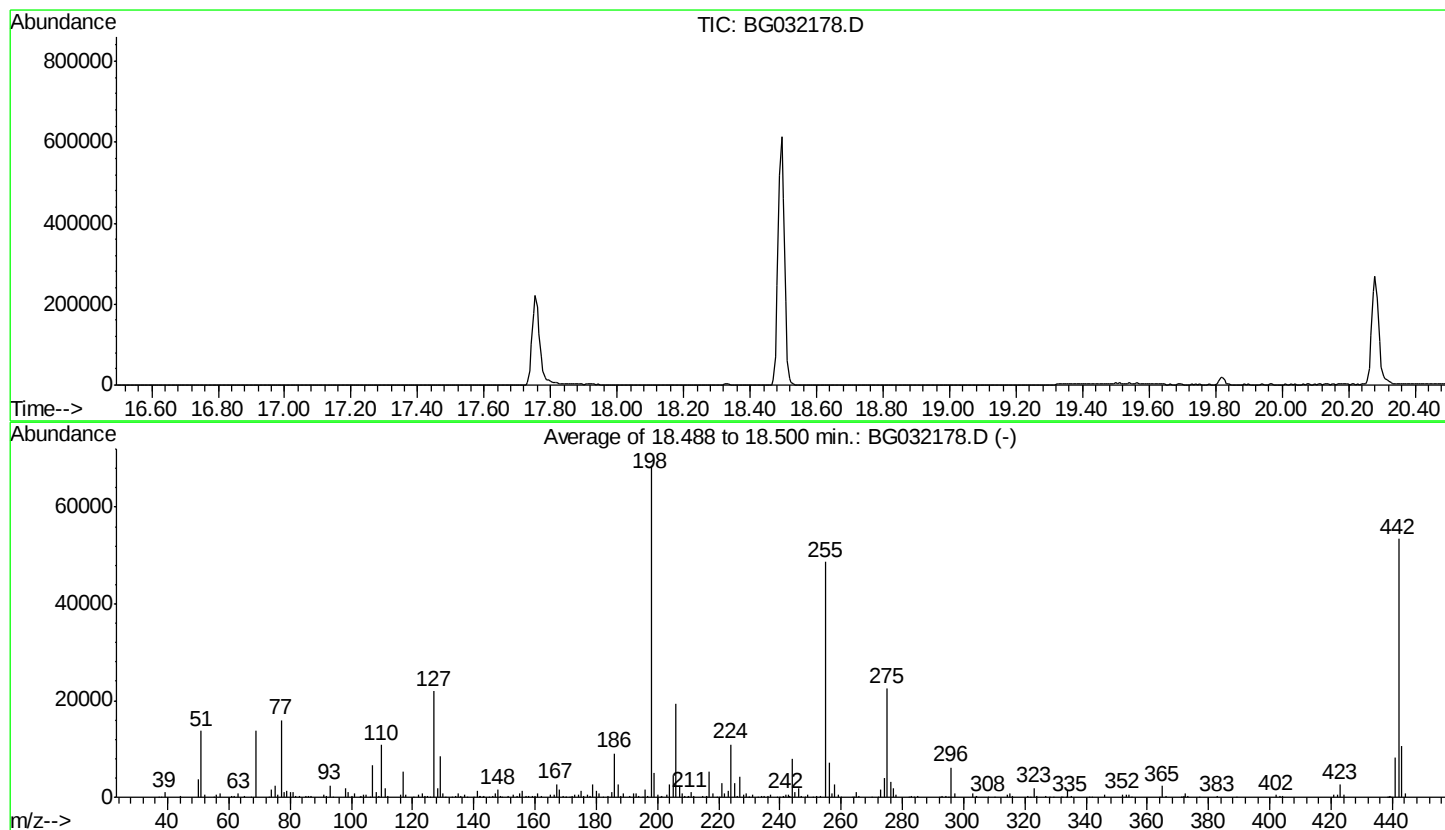

AutoFind: Scans 2587, 2588, 2589; Background Corrected with Scan 2579

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	20.0	13738	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	19.9	13664	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	31.9	21880	PASS
197	198	0.00	2	0.3	178	PASS
198	198	100	100	100.0	68597	PASS
199	198	5	9	7.2	4928	PASS
275	198	10	60	32.7	22432	PASS
365	198	1	100	3.5	2379	PASS
441	442	0.01	24	15.4	8225	PASS
442	198	50	100	77.8	53378	PASS
443	442	15	24	19.7	10505	PASS