
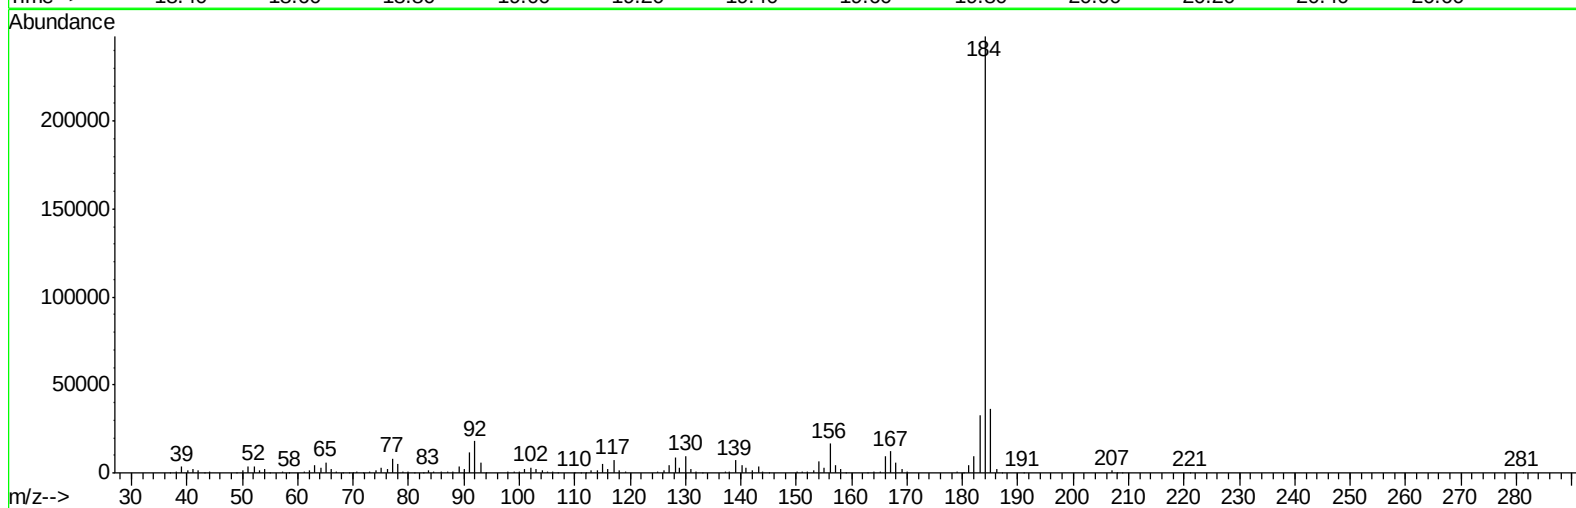


Data File : BG044118.D  
Acq On : 21 Jan 2020 4:10  
Operator : JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 21 07:58:32 2020  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG123019.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Dec 31 13:32:23 2019  
Response via : Initial Calibration

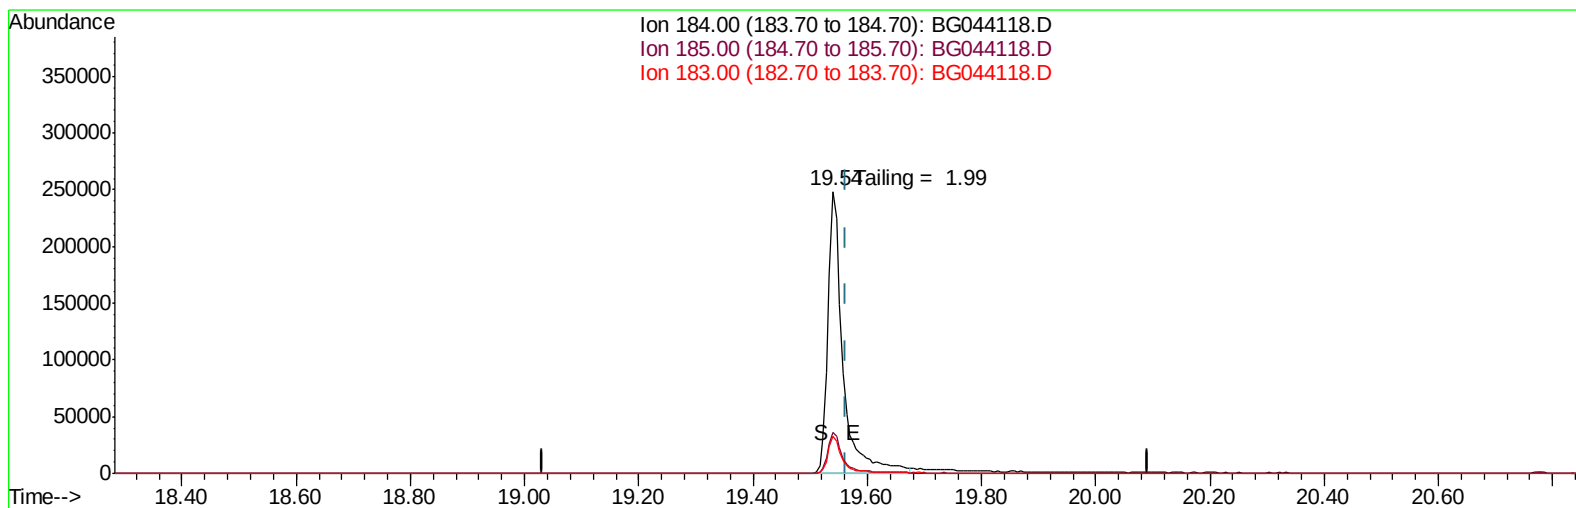

TIC: BG044118.D

(77) Benzidine

19.540min (-0.023) 314795.25ng

response 474755

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 16.70 | 14.74 |
| 183.00 | 13.20 | 13.32 |
| 0.00   | 0.00  | 0.00  |