
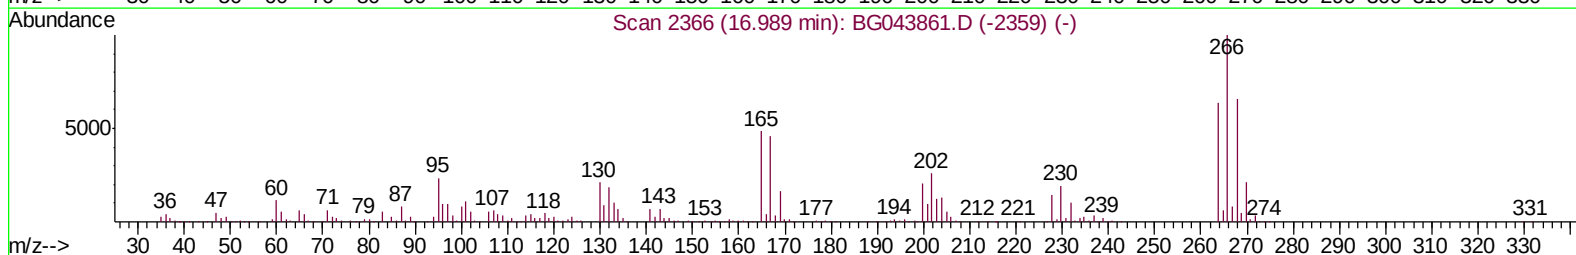
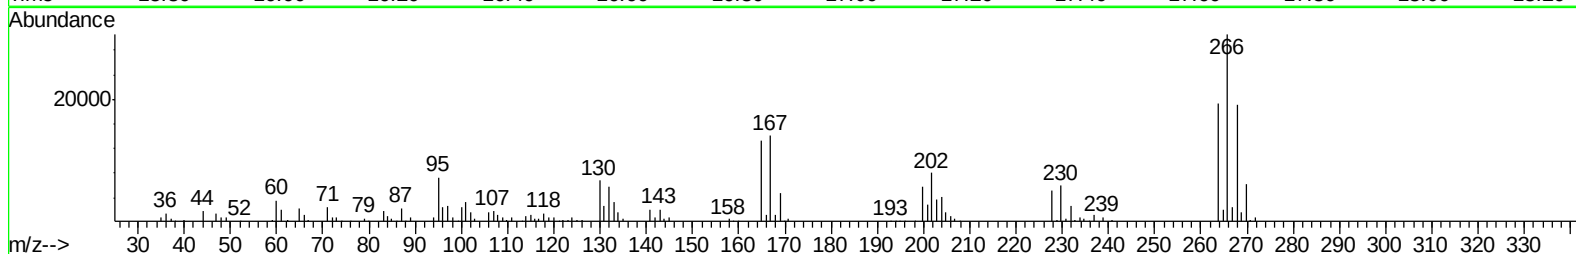


Data File : BG044091.D
Acq On : 20 Jan 2020 9:38
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 21 07:50:44 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG123019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 31 13:32:23 2019
Response via : Initial Calibration

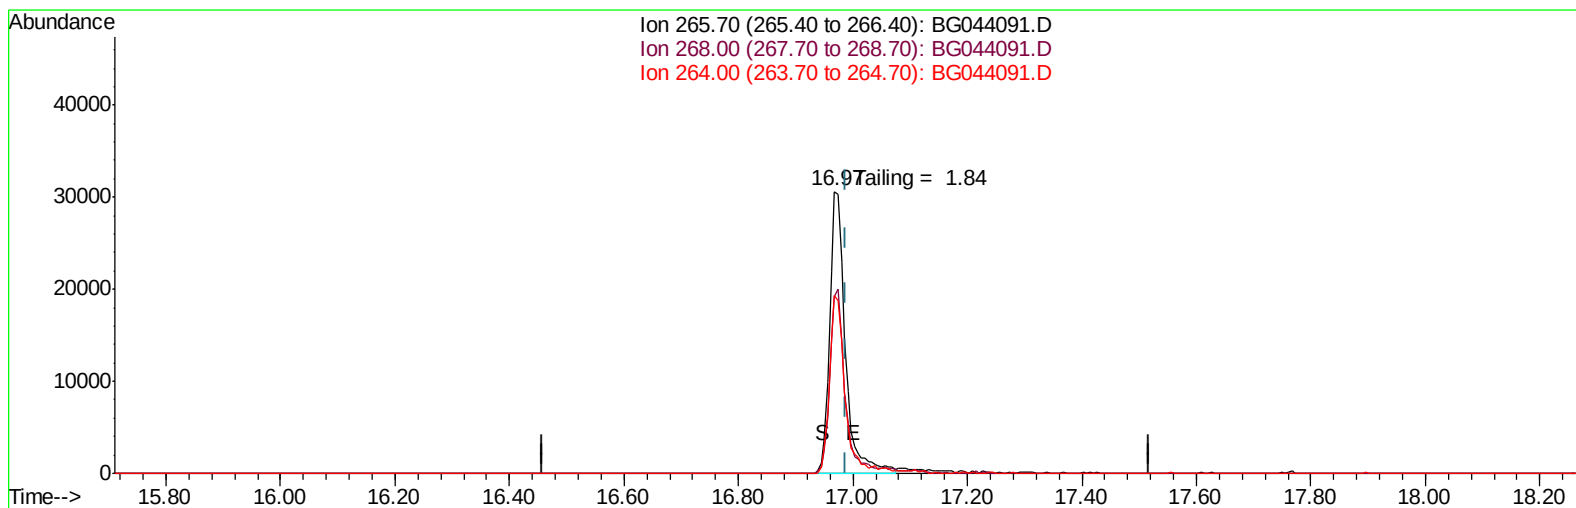

TIC: BG044091.D

(70) Pentachlorophenol (C)




16.968min (-0.021) 27153.66ng

response 58230

Ion	Exp%	Act%
265.70	100	100
268.00	65.80	62.62
264.00	63.50	63.38
0.00	0.00	0.00

Data File : BG044091.D
Acq On : 20 Jan 2020 9:38
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 21 07:50:44 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG123019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 31 13:32:23 2019
Response via : Initial Calibration

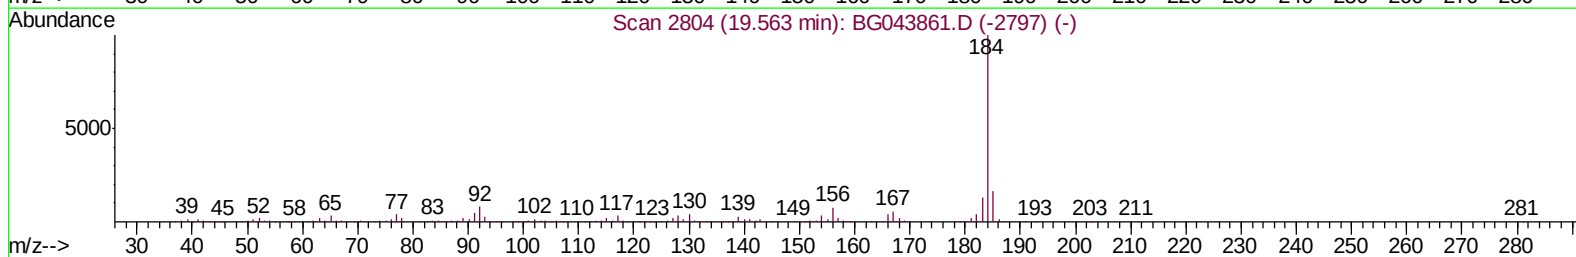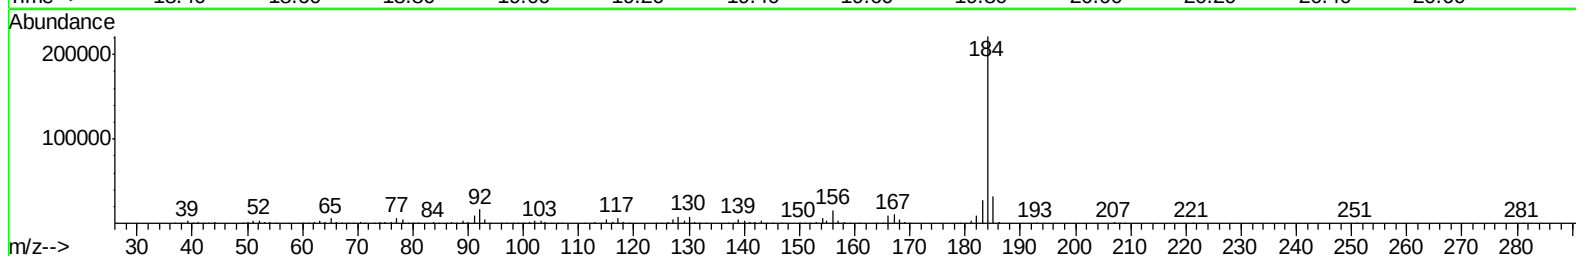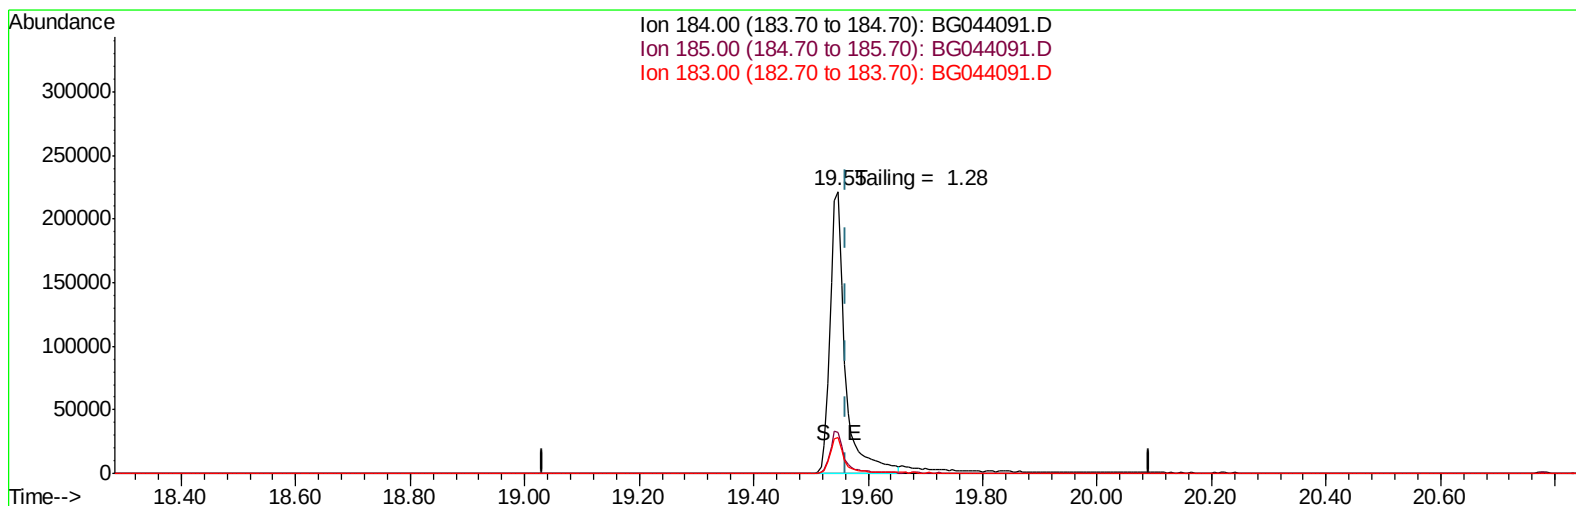

TIC: BG044091.D

(77) Benzidine

19.547min (-0.015) 0.00ng

response 419559

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.61
183.00	13.20	12.58
0.00	0.00	0.00