

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG012020\
 Data File : BG044128.D
 Acq On : 21 Jan 2020 11:28
 Operator : JU
 Sample : L1162-03
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MH-5-(SETTLED)

Quant Time: Jan 21 12:15:25 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG123019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 31 13:32:23 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.93	152	88457	20.00	ng	-0.04
21) Naphthalene-d8	10.73	136	397295	20.00	ng	-0.04
39) Acenaphthene-d10	14.57	164	266565	20.00	ng	-0.03
64) Phenanthrene-d10	17.31	188	528935	20.00	ng	-0.02
76) Chrysene-d12	21.55	240	447620	20.00	ng	-0.04
87) Perylene-d12	24.66	264	498217	20.00	ng	-0.06
System Monitoring Compounds						
5) 2-Fluorophenol	5.51	112	367627	76.31	ng	-0.03
7) Phenol-d6	7.10	99	326321	48.46	ng	-0.02
23) Nitrobenzene-d5	9.09	82	633415	85.29	ng	-0.04
42) 2,4,6-Tribromophenol	16.05	330	409147	146.67	ng	-0.03
45) 2-Fluorobiphenyl	13.19	172	1463603	99.48	ng	-0.03
79) Terphenyl-d14	19.93	244	1857815	106.74	ng	-0.03
Target Compounds						
10) Phenol	7.12	94	26665	3.843	ng	98
50) Dimethylphthalate	14.02	163	157269	8.309	ng	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG012020\
Data File : BG044128.D
Acq On : 21 Jan 2020 11:28
Operator : JU
Sample : L1162-03
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MH-5-(SETTLED)

Quant Time: Jan 21 12:15:25 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG123019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 31 13:32:23 2019
Response via : Initial Calibration

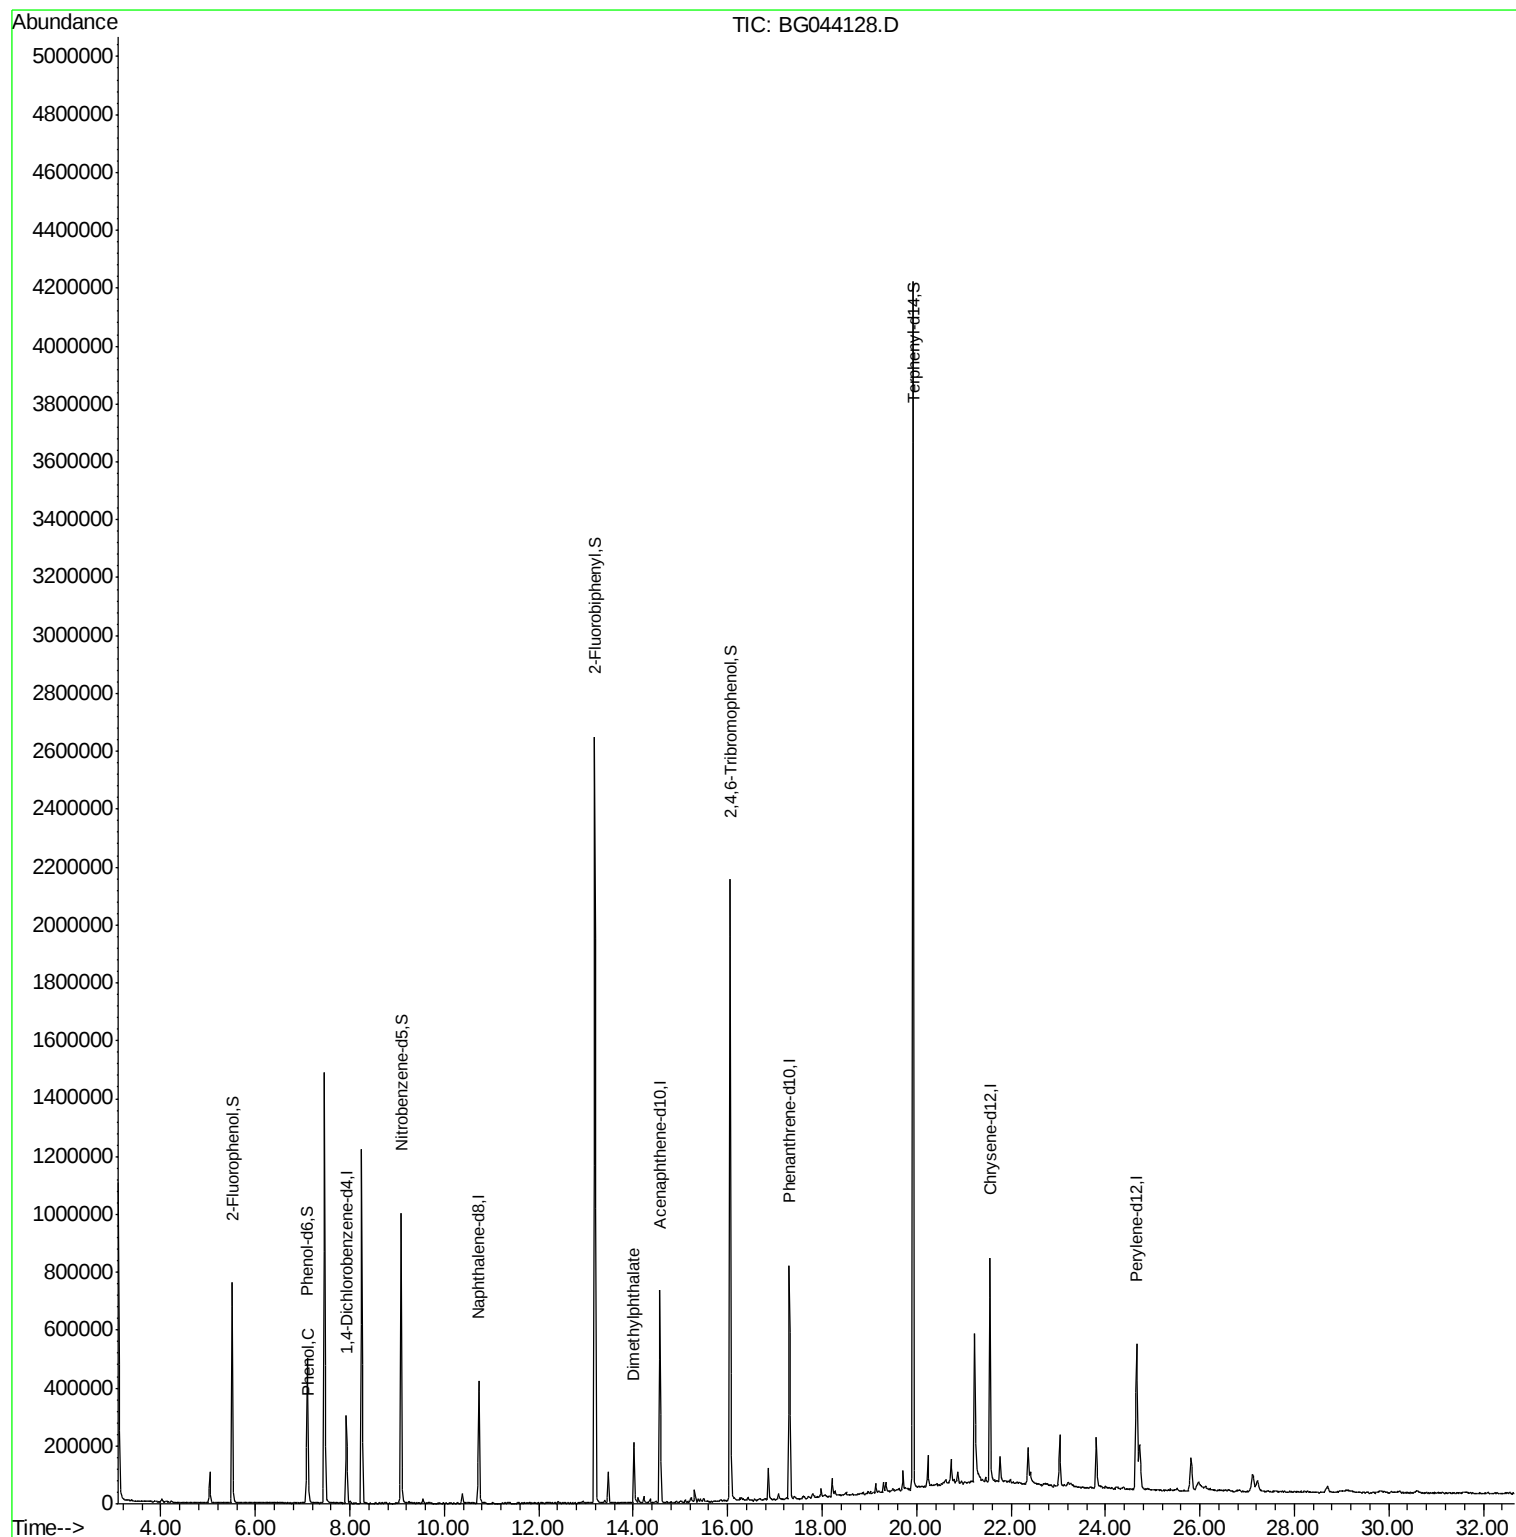







#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.93 min Scan# 824
Delta R.T. -0.04 min
Lab File: BG044128.D
Acq: 21 Jan 2020 11:28

Instrument :
BNA_G
ClientSampleId :
MH-5-(SETTLED)




Tot Ion	Ratio	Lower	Upper
152	100		
150	159.4	127.0	190.4
115	60.8	47.8	71.8

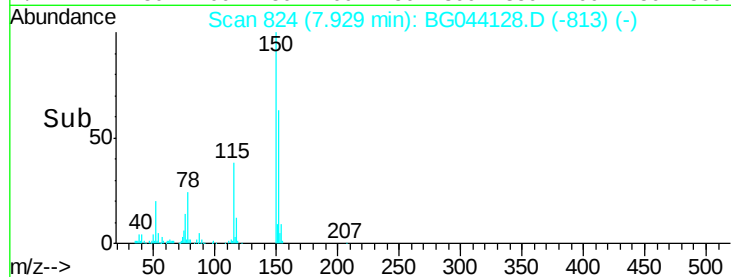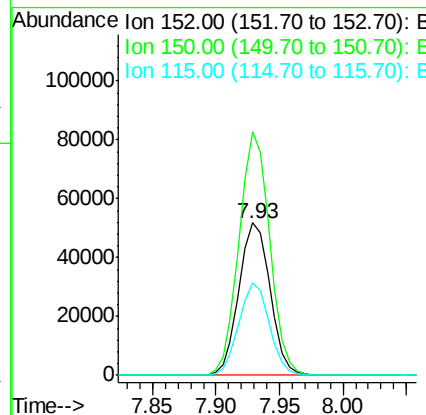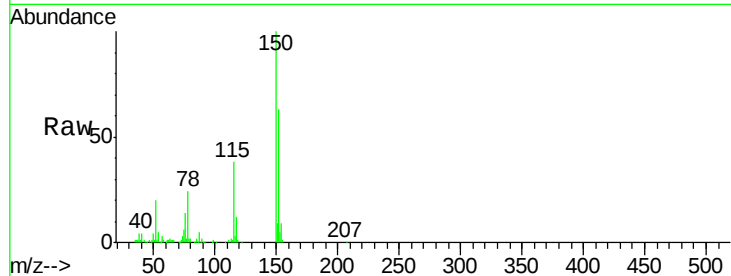


#5

2-Fluorophenol
Concen: 76.309 ng
RT: 5.51 min Scan# 412
Delta R.T. -0.03 min
Lab File: BG044128.D
Acq: 21 Jan 2020 11:28

Tgt Ion	Ratio	Lower	Upper
112	100		
64	55.9	47.8	71.6
63	29.2	24.3	36.5

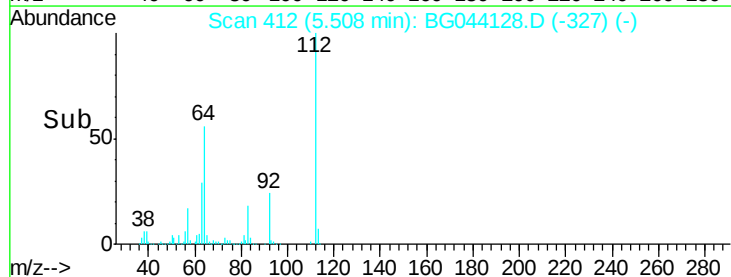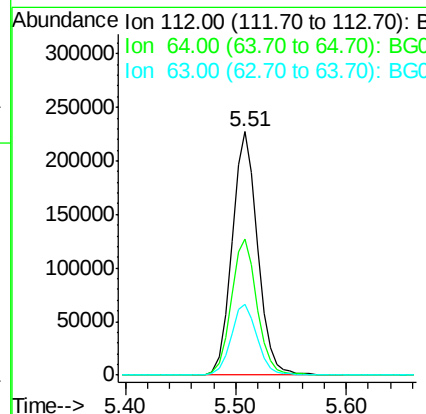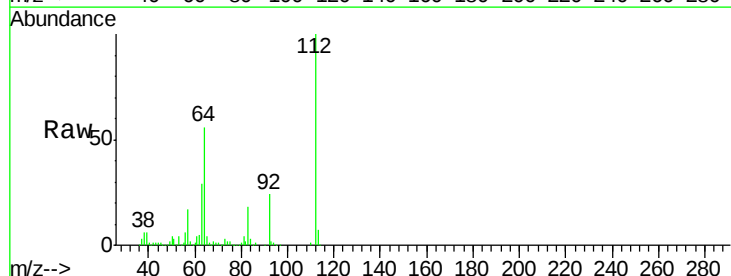

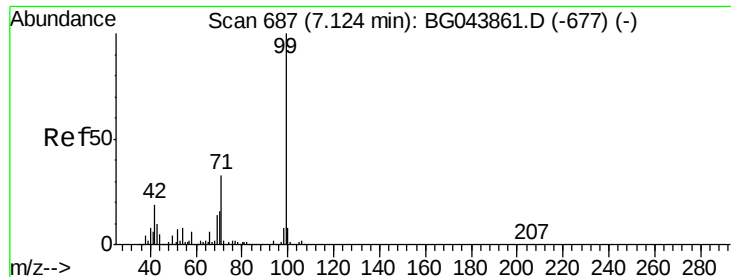

#7

Phenol-d6

Concen: 48.458 ng

RT: 7.10 min Scan# 683

Delta R.T. -0.02 min

Lab File: BG044128.D

Acq: 21 Jan 2020 11:28

Instrument :

BNA_G

ClientSampleId :

MH-5-(SETTLED)


Tot Ion: 99 Resp: 326321

Ion Ratio Lower Upper




99 100

42 16.8 14.9 22.3

71 31.7 26.4 39.6



Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

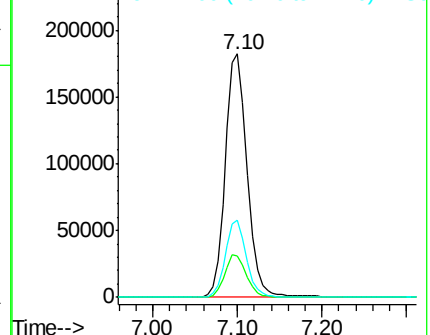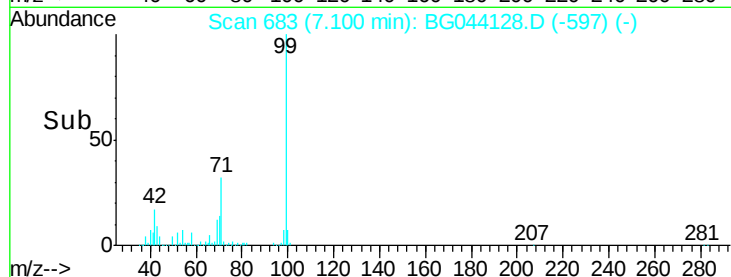

#10

Phenol

Concen: 3.843 ng

RT: 7.12 min Scan# 687

Delta R.T. -0.03 min

Lab File: BG044128.D

Acq: 21 Jan 2020 11:28


Tgt Ion: 94 Resp: 26665

Ion Ratio Lower Upper



94 100

65 26.2 8.1 48.1

66 35.0 15.6 55.6



Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC

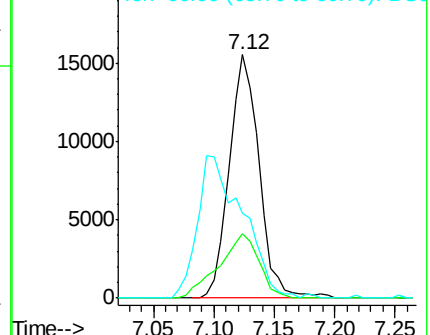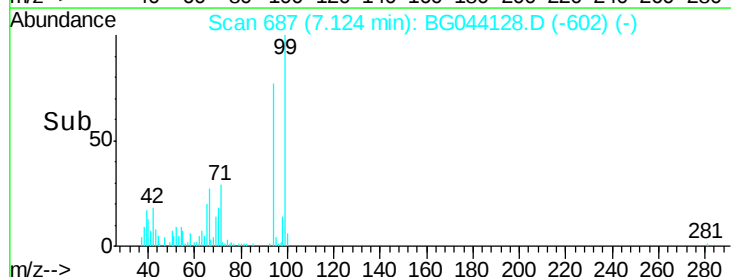







#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.73 min Scan# 1301
Delta R.T. -0.04 min
Lab File: BG044128.D
Acq: 21 Jan 2020 11:28

Instrument :
BNA_G
ClientSampleId :
MH-5-(SETTLED)

Tot Ion:136	Resp:	397295
Ion Ratio	Lower	Upper
136 100		
137 11.0	8.8	13.2
54 8.0	7.0	10.4
68 5.7	4.9	7.3

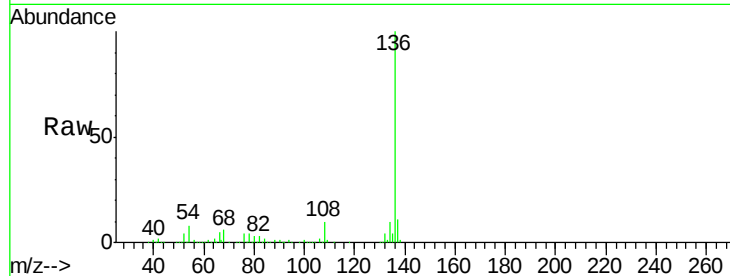


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

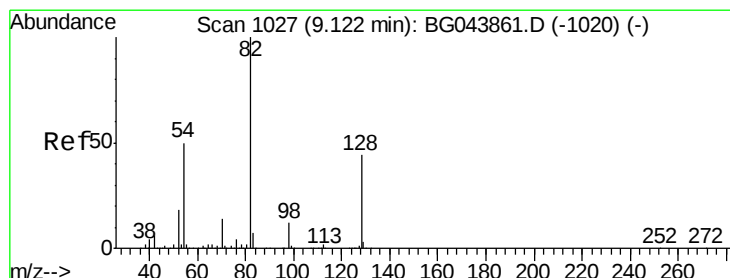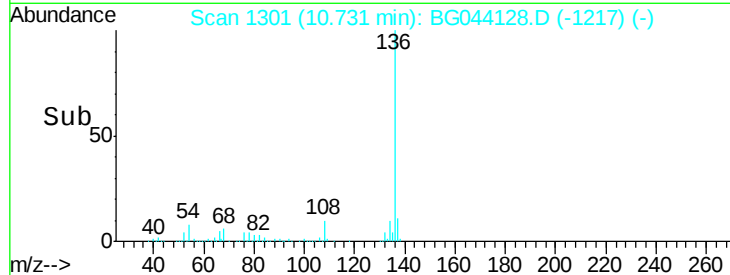
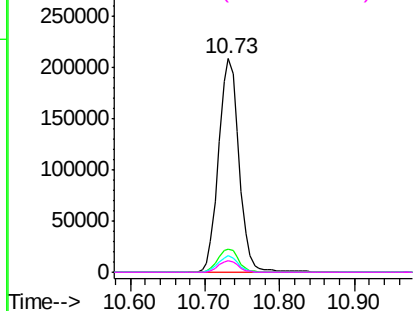



#23
Nitrobenzene-d5
Concen: 85.290 ng
RT: 9.09 min Scan# 1021
Delta R.T. -0.04 min
Lab File: BG044128.D
Acq: 21 Jan 2020 11:28

Tgt	Ion: 82	Resp:	633415
Ion	Ratio	Lower	Upper
82	100		
128	45.8	35.1	52.7
54	49.1	40.1	60.1

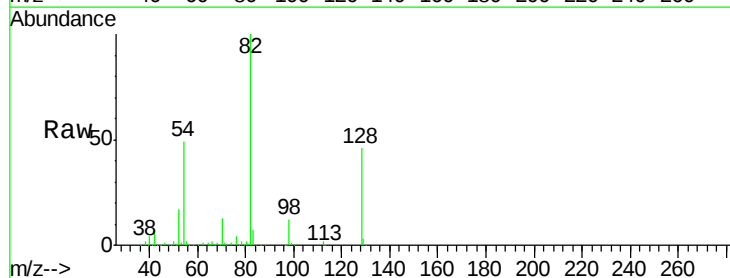

Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BGC



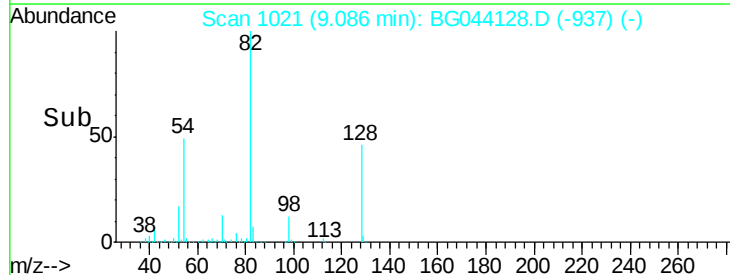
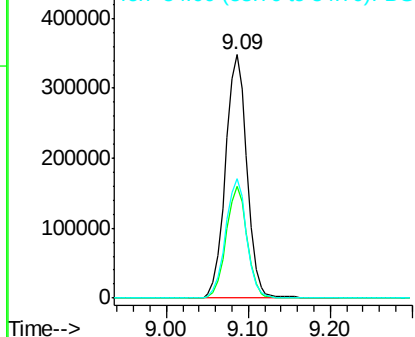


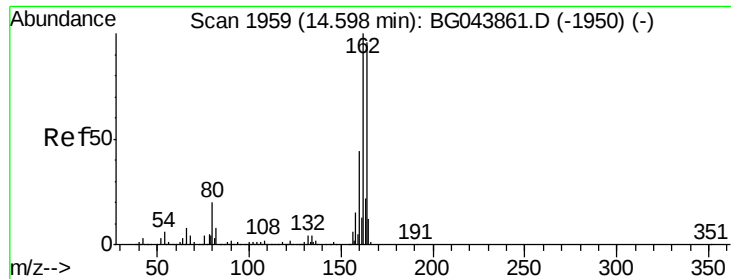

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.57 min Scan# 1954
Delta R.T. -0.03 min
Lab File: BG044128.D
Acq: 21 Jan 2020 11:28




Instrument :
BNA_G
ClientSampleId :
MH-5-(SETTLED)

Tot Ion	Ratio	Lower	Upper
164	100		
162	104.7	83.0	124.4
160	44.9	36.1	54.1

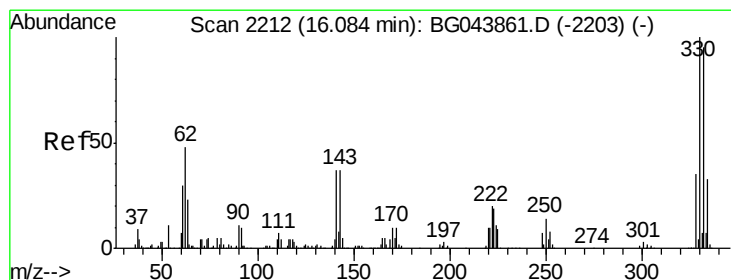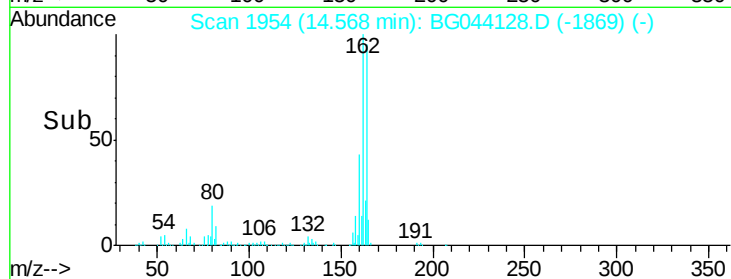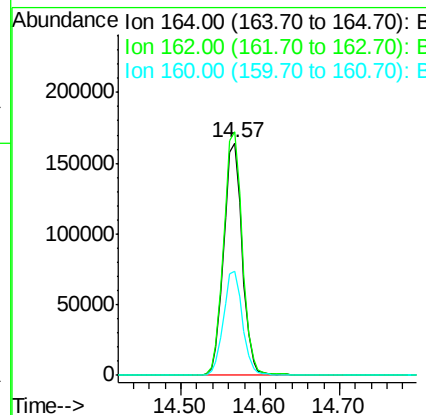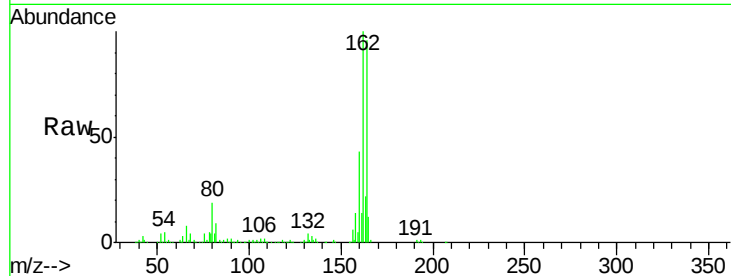

#42
2,4,6-Tribromophenol
Concen: 146.671 ng
RT: 16.05 min Scan# 2207
Delta R.T. -0.03 min
Lab File: BG044128.D
Acq: 21 Jan 2020 11:28

Tgt Ion	Ratio	Lower	Upper
330	100		
332	96.1	77.2	115.8
141	39.3	33.1	49.7

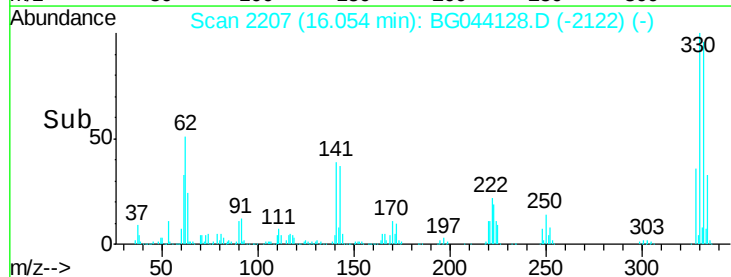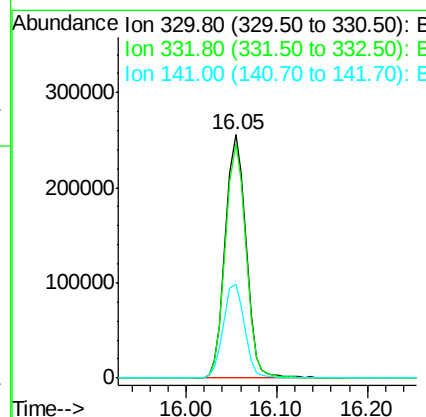



#45

2-Fluorobiphenyl

Concen: 99.477 ng

RT: 13.19 min Scan# 1720

Delta R.T. -0.03 min

Lab File: BG044128.D

Acq: 21 Jan 2020 11:28

Instrument :


BNA_G

ClientSampleId :

MH-5-(SETTLED)

Tot Ion:172 Resp: 1463603

Ion	Ratio	Lower	Upper
172	100		
171	40.3	35.8	53.8
170	27.5	24.2	36.4




Abundance

Ion 172.00 (171.70 to 172.70): E


Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

Time-->

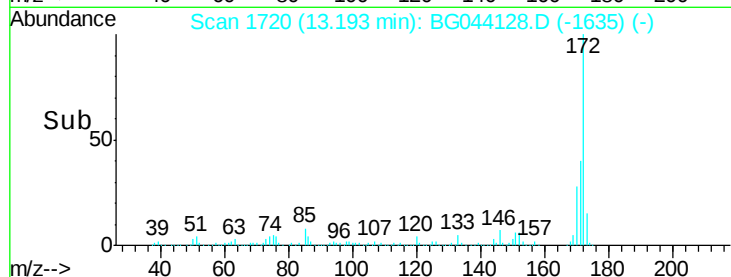

Time-->



#50

Dimethylphthalate

Concen: 8.309 ng

RT: 14.02 min Scan# 1860


Delta R.T. -0.04 min

Lab File: BG044128.D

Acq: 21 Jan 2020 11:28

Tgt Ion:163 Resp: 157269

Ion	Ratio	Lower	Upper
163	100		
194	4.0	3.7	5.5
164	10.2	9.3	13.9




Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

Time-->

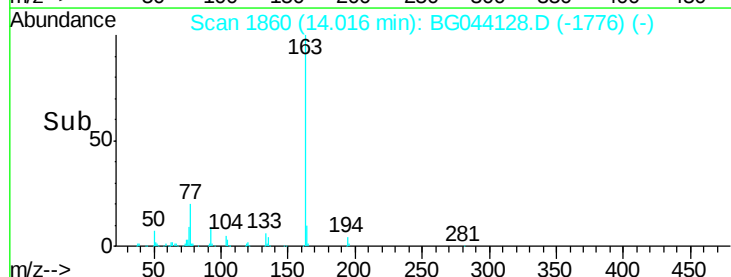

Time-->



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.31 min Scan# 2421

Delta R.T. -0.02 min

Lab File: BG044128.D

Acq: 21 Jan 2020 11:28

Instrument :

BNA_G

ClientSampleId :

MH-5-(SETTLED)


Tot Ion:188 Resp: 528935

Ion Ratio Lower Upper

188 100

94 9.2 7.9 11.9




80 9.8 8.2 12.4

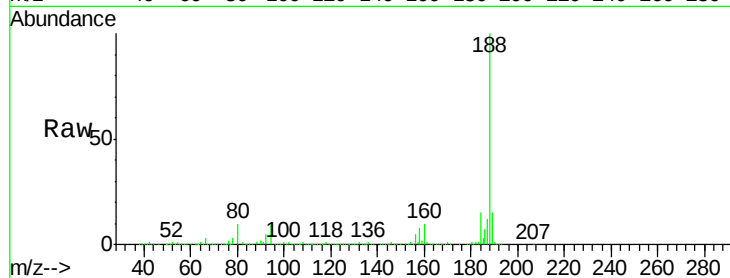

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BGC

Ion 80.00 (79.70 to 80.70): BGC

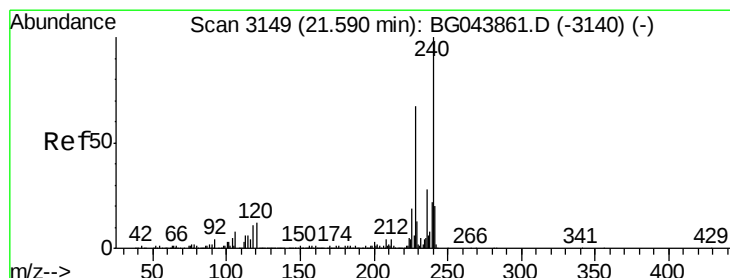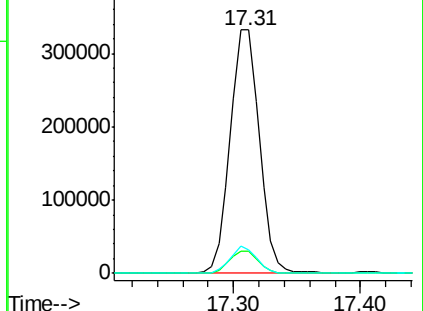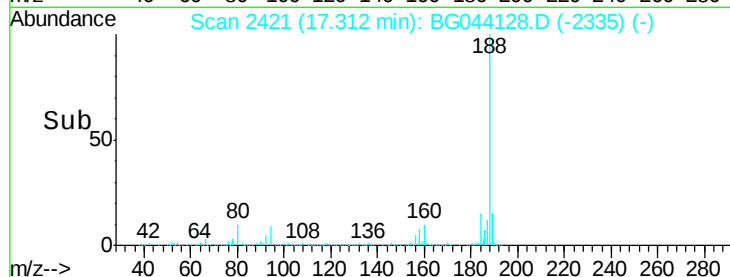

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.55 min Scan# 3143

Delta R.T. -0.04 min

Lab File: BG044128.D

Acq: 21 Jan 2020 11:28


Tgt Ion:240 Resp: 447620

Ion Ratio Lower Upper

240 100

120 11.5 9.6 14.4



236 27.7 22.2 33.2

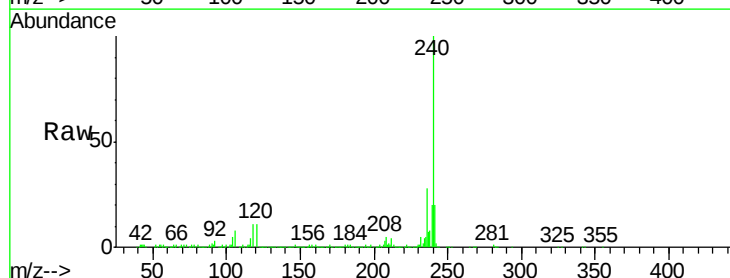


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

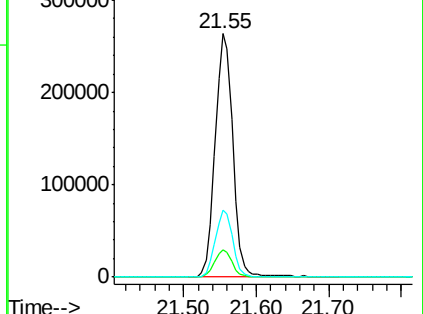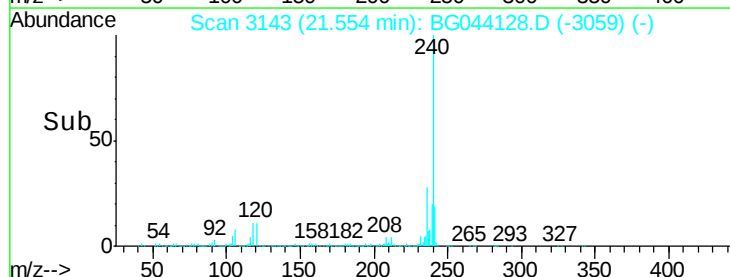

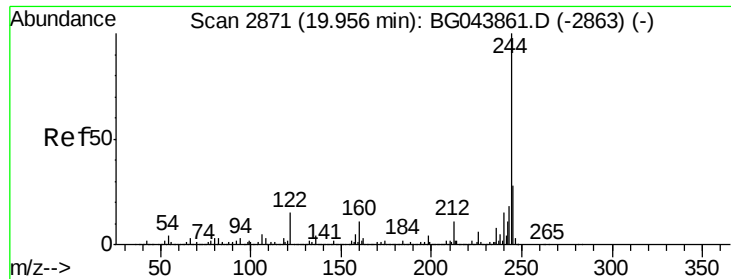

#79

Terphenyl-d14

Concen: 106.737 ng

RT: 19.93 min Scan# 2866

Delta R.T. -0.03 min

Lab File: BG044128.D

Acq: 21 Jan 2020 11:28

Instrument :

BNA_G

ClientSampleId :

MH-5-(SETTLED)


Tot Ion:244 Resp: 1857815

Ion Ratio Lower Upper

244 100

212 9.6 8.6 13.0




122 13.1 11.9 17.9



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

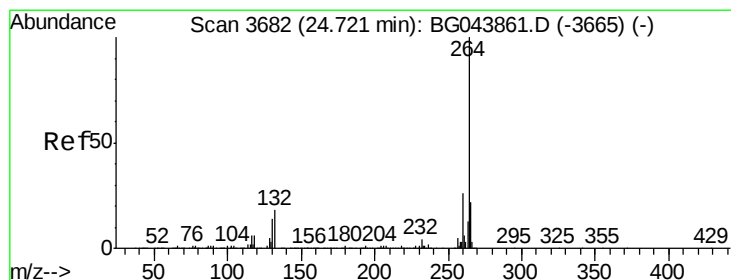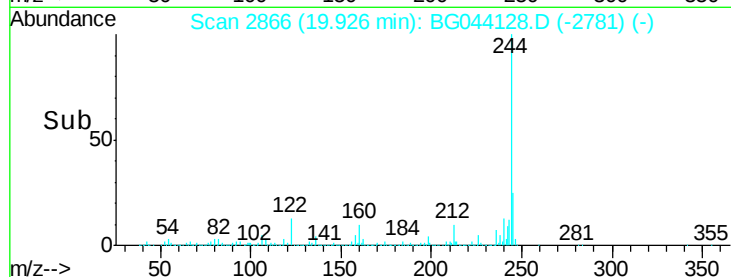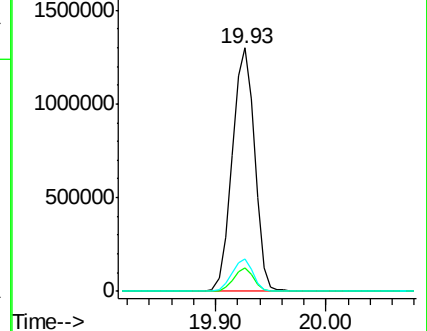

#87

Perylene-d12

Concen: 20.000 ng

RT: 24.66 min Scan# 3672

Delta R.T. -0.06 min

Lab File: BG044128.D

Acq: 21 Jan 2020 11:28


Tgt Ion:264 Resp: 498217

Ion Ratio Lower Upper

264 100

260 25.1 20.4 30.6

265 22.0 17.4 26.2



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

