


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG012020\  
 Data File : BG044099.D  
 Acq On : 20 Jan 2020 15:45  
 Operator : JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG123019.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Tue Dec 31 13:32:23 2019

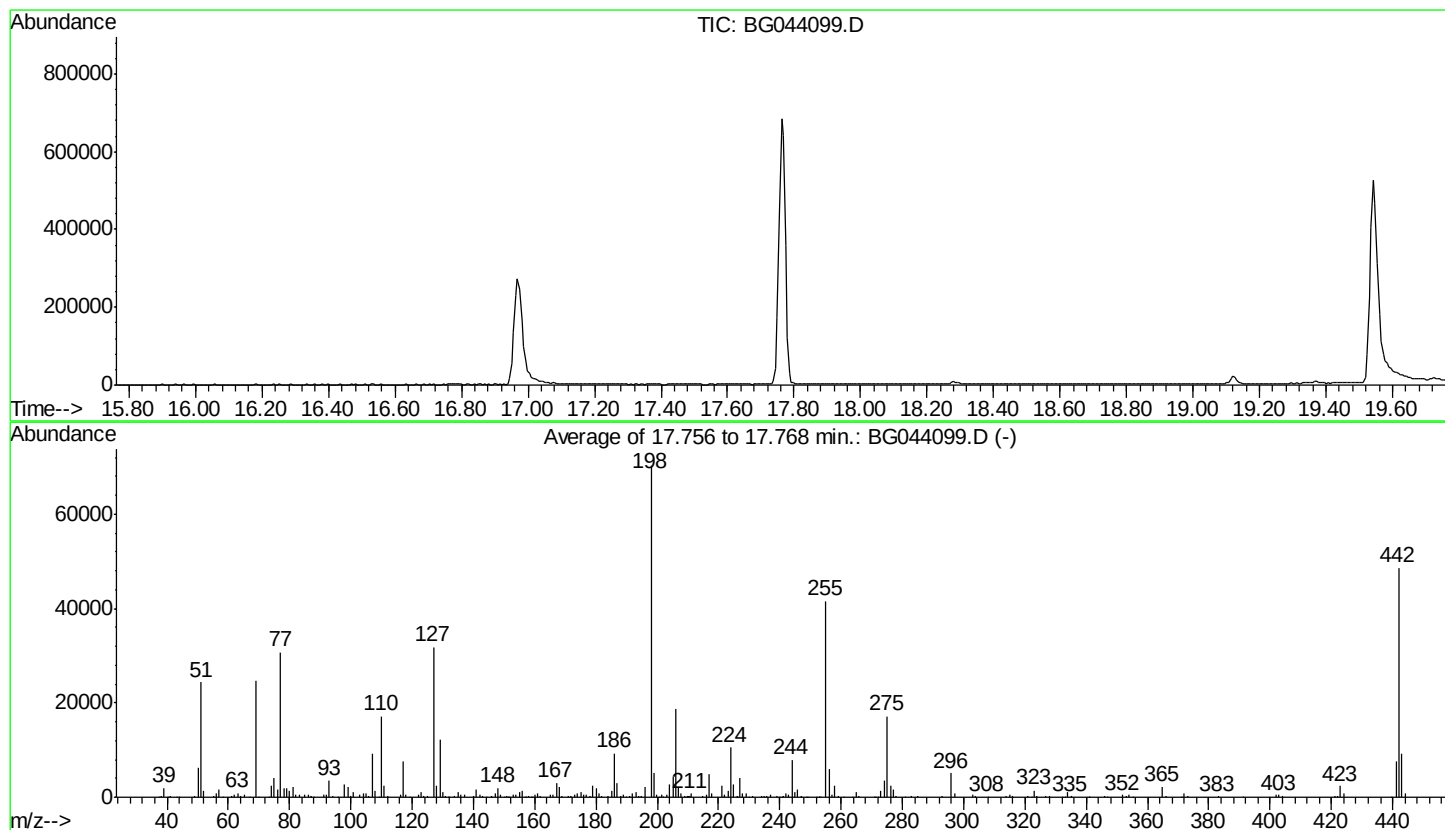

AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2490

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 34.7      | 24376   | PASS             |
| 68          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 69          | 198          | 0.00         | 100          | 35.3      | 24810   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.3       | 78      | PASS             |
| 127         | 198          | 10           | 80           | 45.2      | 31784   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 70293   | PASS             |
| 199         | 198          | 5            | 9            | 7.2       | 5049    | PASS             |
| 275         | 198          | 10           | 60           | 24.5      | 17211   | PASS             |
| 365         | 198          | 1            | 100          | 3.3       | 2303    | PASS             |
| 441         | 198          | 0.01         | 100          | 10.7      | 7518    | PASS             |
| 442         | 198          | 50           | 100          | 69.2      | 48674   | PASS             |
| 443         | 442          | 15           | 24           | 19.2      | 9322    | PASS             |